

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112224\
 Data File : BP023300.D
 Acq On : 22 Nov 2024 12:40
 Operator : RC/JU
 Sample : P4930-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BG440

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023300.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.099	15	19	23	rBV	45754	66148	1.90%	0.255%
2	3.134	23	25	29	rVB	18101	19102	0.55%	0.074%
3	3.564	95	98	112	rBV	27997	67457	1.94%	0.260%
4	3.852	143	147	153	rVB4	5940	10780	0.31%	0.042%
5	4.275	214	219	225	rVB	9972	15269	0.44%	0.059%
6	4.363	229	234	242	rVB	51887	79030	2.28%	0.305%
7	6.705	627	632	636	rBV	6306	8494	0.24%	0.033%
8	6.781	639	645	662	rBV	69684	166638	4.80%	0.642%
9	6.916	662	668	680	rVB	258079	442614	12.74%	1.705%
10	7.110	695	701	725	rVB	318164	557125	16.04%	2.147%
11	7.563	771	778	789	rBV	280730	495899	14.28%	1.911%
12	8.275	891	899	923	rBV	229669	496229	14.29%	1.912%
13	8.704	965	972	988	rBV	322023	638050	18.37%	2.458%
14	9.087	1033	1037	1047	rVB5	4845	7913	0.23%	0.030%
15	9.410	1086	1092	1110	rBV	274638	562285	16.19%	2.167%
16	9.969	1180	1187	1214	rBV	369063	817066	23.53%	3.148%
17	10.310	1238	1245	1256	rVB	376005	655879	18.88%	2.527%
18	10.463	1265	1271	1286	rBV	200790	468600	13.49%	1.806%
19	11.557	1451	1457	1463	rVB10	3082	6829	0.20%	0.026%
20	11.922	1512	1519	1524	rBV5	4404	9781	0.28%	0.038%
21	12.787	1660	1666	1674	rBV5	2206	6803	0.20%	0.026%
22	13.587	1795	1802	1815	rBV	1125965	1378718	39.70%	5.312%
23	13.875	1840	1851	1859	rBV	994944	1419845	40.88%	5.471%
24	14.181	1895	1903	1914	rBV	582445	947478	27.28%	3.651%
25	14.528	1956	1962	1966	rBV3	26304	63264	1.82%	0.244%
26	15.204	2068	2077	2089	rBV	1116200	1934992	55.71%	7.456%
27	15.357	2097	2103	2115	rBV	367179	603329	17.37%	2.325%
28	15.586	2134	2142	2148	rBV2	18832	36648	1.06%	0.141%
29	16.145	2231	2237	2244	rVB2	11174	19527	0.56%	0.075%
30	16.304	2259	2264	2268	rBV7	2285	3799	0.11%	0.015%
31	16.786	2343	2346	2353	rVB6	2842	5465	0.16%	0.021%
32	16.998	2376	2382	2393	rVV	793982	1263921	36.39%	4.870%
33	17.104	2393	2400	2414	rVV	1647290	2378607	68.49%	9.165%
34	17.692	2498	2500	2507	rVB8	4303	6533	0.19%	0.025%
35	17.933	2536	2541	2551	rBV3	68233	118495	3.41%	0.457%
36	18.010	2551	2554	2562	rVB4	7042	12966	0.37%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112224\
Data File : BP023300.D
Acq On : 22 Nov 2024 12:40
Operator : RC/JU
Sample : P4930-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG440

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	18.233	2589	2592	2596	rBV6	3342	4209	0.12%	0.016%
38	18.810	2685	2690	2693	rBV6	6349	12916	0.37%	0.050%
39	19.027	2723	2727	2737	rVB3	26189	41943	1.21%	0.162%
40	19.110	2737	2741	2745	rBV2	16875	30269	0.87%	0.117%
41	19.204	2754	2757	2761	rVB3	15667	19689	0.57%	0.076%
42	19.280	2764	2770	2779	rBV5	45948	96479	2.78%	0.372%
43	19.422	2792	2794	2797	rVB3	6154	5560	0.16%	0.021%
44	19.480	2798	2804	2819	rVV	1866882	3021594	87.00%	11.643%
45	20.210	2925	2928	2934	rVB8	19166	24520	0.71%	0.094%
46	21.439	3131	3137	3150	rBV2	867712	1604943	46.21%	6.184%
47	24.439	3638	3647	3662	rBV	1311480	3473159	100.00%	13.383%
48	24.662	3677	3685	3706	rVB	645956	1826106	52.58%	7.036%




Sum of corrected areas: 25952965

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112224\
Data File : BP023300.D
Acq On : 22 Nov 2024 12:40
Operator : RC/JU
Sample : P4930-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG440

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

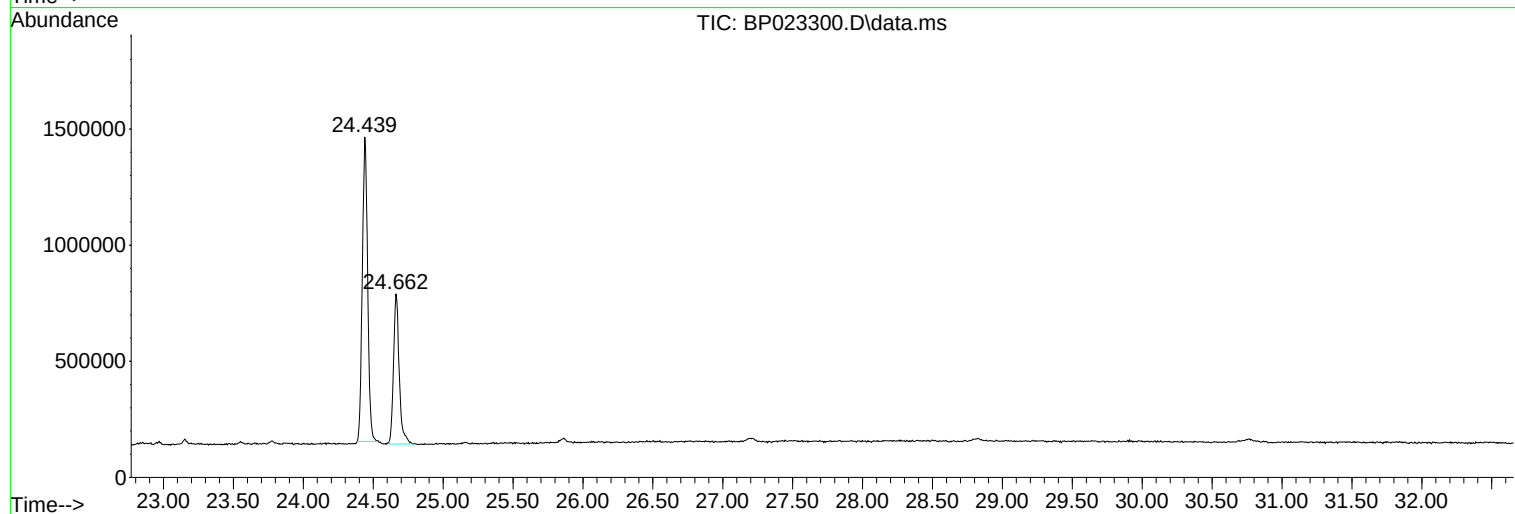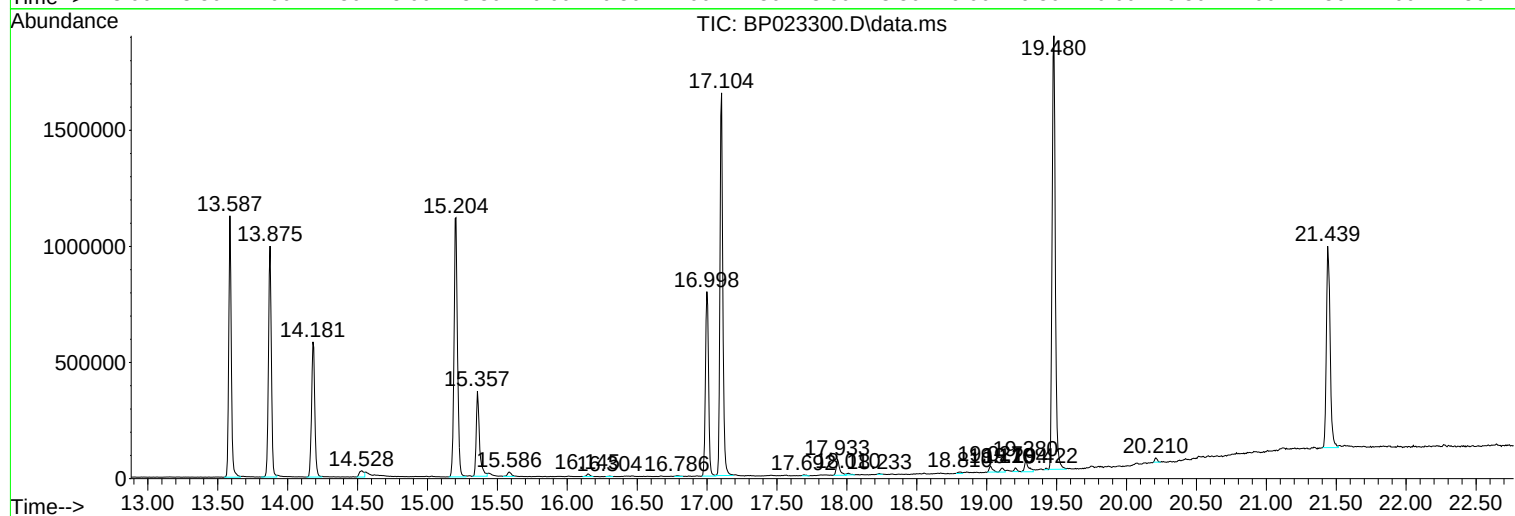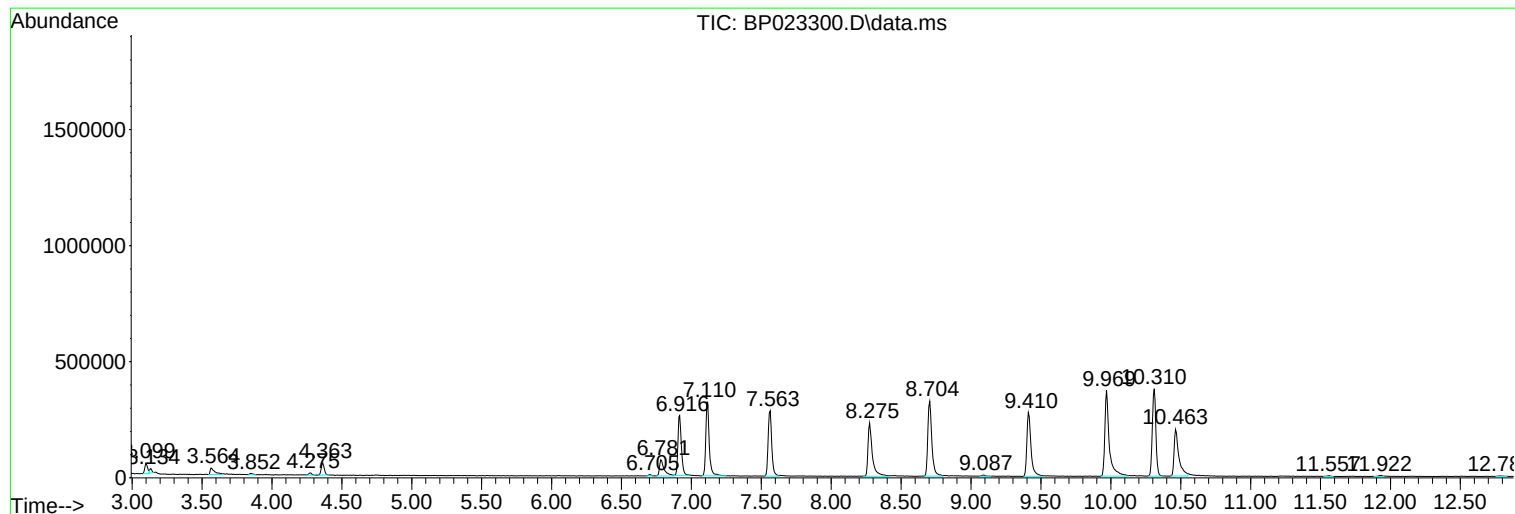

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112224\
Data File : BP023300.D
Acq On : 22 Nov 2024 12:40
Operator : RC/JU
Sample : P4930-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG440

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112224\
Data File : BP023300.D
Acq On : 22 Nov 2024 12:40
Operator : RC/JU
Sample : P4930-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG440

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
