

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112224\
 Data File : BP023301.D
 Acq On : 22 Nov 2024 13:21
 Operator : RC/JU
 Sample : P4930-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BG441

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023301.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.099	14	19	23	rBV	39218	60771	1.65%	0.215%
2	3.134	23	25	28	rVV	22606	26679	0.73%	0.094%
3	3.170	28	31	37	rVB5	10023	15326	0.42%	0.054%
4	3.564	95	98	111	rBV	29787	69886	1.90%	0.247%
5	3.852	143	147	152	rBV2	4670	6889	0.19%	0.024%
6	4.269	214	218	225	rVB	12214	18559	0.51%	0.066%
7	4.364	228	234	244	rVB	51067	83794	2.28%	0.296%
8	6.699	626	631	636	rBV3	9046	16844	0.46%	0.059%
9	6.781	639	645	661	rVV	77258	191567	5.22%	0.677%
10	6.911	662	667	689	rVV	305941	513246	13.97%	1.813%
11	7.111	693	701	726	rVV	325361	612556	16.68%	2.164%
12	7.563	770	778	788	rBV	342304	540952	14.73%	1.911%
13	7.634	788	790	798	rVB8	5063	9266	0.25%	0.033%
14	8.275	893	899	917	rBV	269968	552774	15.05%	1.952%
15	8.705	965	972	994	rBV	405612	701887	19.11%	2.479%
16	8.881	994	1002	1007	rBV	3543	10144	0.28%	0.036%
17	9.081	1033	1036	1041	rVB4	6155	9311	0.25%	0.033%
18	9.416	1086	1093	1111	rBV	355815	620688	16.90%	2.192%
19	9.963	1177	1186	1212	rBV	368246	917746	24.99%	3.242%
20	10.310	1237	1245	1259	rVB	407473	700317	19.07%	2.474%
21	10.469	1264	1272	1293	rBV	258661	614921	16.74%	2.172%
22	11.210	1393	1398	1400	rBV5	1938	3736	0.10%	0.013%
23	11.557	1454	1457	1463	rVB3	4385	5872	0.16%	0.021%
24	11.934	1515	1521	1531	rVB6	5264	13217	0.36%	0.047%
25	13.598	1797	1804	1817	rBV	1093605	1544040	42.04%	5.454%
26	13.881	1840	1852	1864	rBV	1002416	1554547	42.33%	5.491%
27	14.187	1895	1904	1916	rBV	663689	1039493	28.30%	3.672%
28	14.516	1953	1960	1961	rBV	27556	41755	1.14%	0.147%
29	14.687	1986	1989	1995	rVB8	5698	9360	0.25%	0.033%
30	15.192	2067	2075	2087	rBV	1204807	2141851	58.32%	7.565%
31	15.298	2090	2093	2097	rVB5	3410	4200	0.11%	0.015%
32	15.357	2097	2103	2115	rBV	406479	688432	18.74%	2.432%
33	15.445	2115	2118	2122	rVB4	10154	15293	0.42%	0.054%
34	15.581	2137	2141	2152	rVB2	11839	21749	0.59%	0.077%
35	16.151	2234	2238	2244	rVB5	6751	11722	0.32%	0.041%
36	16.416	2279	2283	2288	rBV9	3171	5111	0.14%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112224\
 Data File : BP023301.D
 Acq On : 22 Nov 2024 13:21
 Operator : RC/JU
 Sample : P4930-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BG441

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

37	16.786	2344	2346	2350	rVV5	3054	3804	0.10%	0.013%
38	16.992	2374	2381	2393	rBV	853756	1364499	37.15%	4.820%
39	17.104	2393	2400	2415	rBV	1651310	2523424	68.71%	8.913%
40	17.686	2493	2499	2505	rVB10	5386	10941	0.30%	0.039%
41	17.798	2516	2518	2525	rBV8	3991	8777	0.24%	0.031%
42	17.933	2536	2541	2550	rBV2	71881	123024	3.35%	0.435%
43	18.233	2589	2592	2593	rBV3	3949	4055	0.11%	0.014%
44	19.033	2723	2728	2732	rBV4	26526	41423	1.13%	0.146%
45	19.104	2737	2740	2744	rBV	20112	28931	0.79%	0.102%
46	19.198	2754	2756	2762	rVB3	17194	21787	0.59%	0.077%
47	19.275	2765	2769	2775	rBV5	31147	55252	1.50%	0.195%
48	19.428	2792	2795	2798	rBV5	7637	11157	0.30%	0.039%
49	19.480	2798	2804	2819	rVV	2405738	3349774	91.21%	11.832%
50	21.445	3132	3138	3153	rBV	984866	1738673	47.34%	6.141%
51	24.457	3641	3650	3665	rVB	1397606	3672734	100.00%	12.972%
52	24.680	3679	3688	3710	rVB	646125	1959014	53.34%	6.919%




Sum of corrected areas: 28311770

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112224\
Data File : BP023301.D
Acq On : 22 Nov 2024 13:21
Operator : RC/JU
Sample : P4930-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG441

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

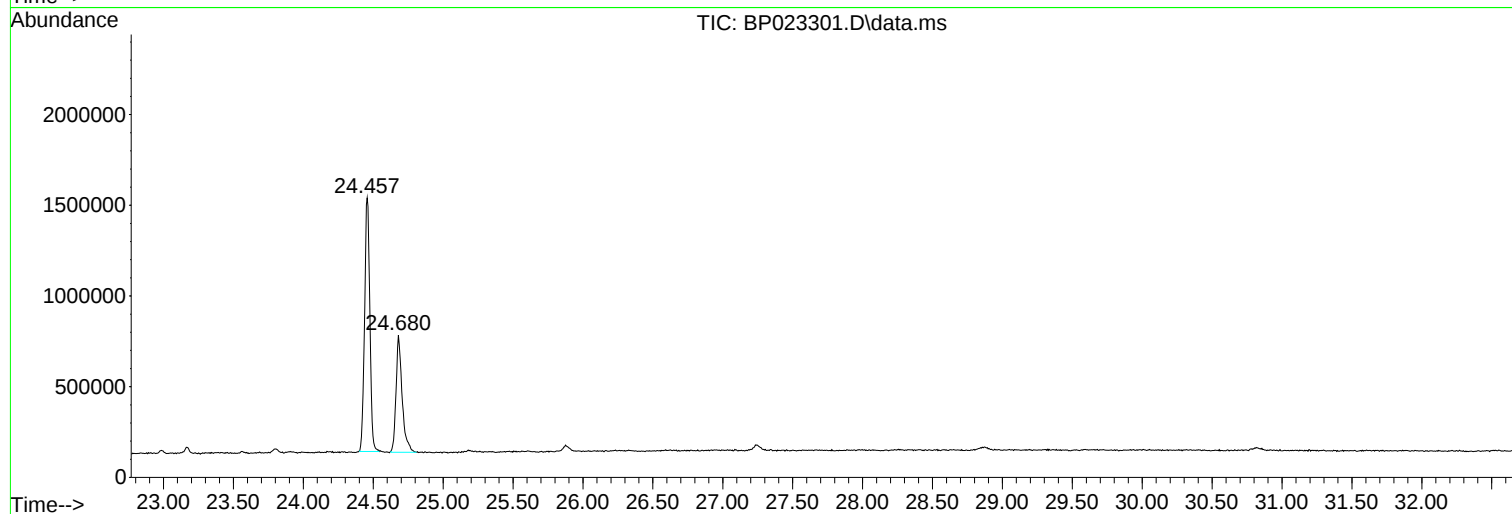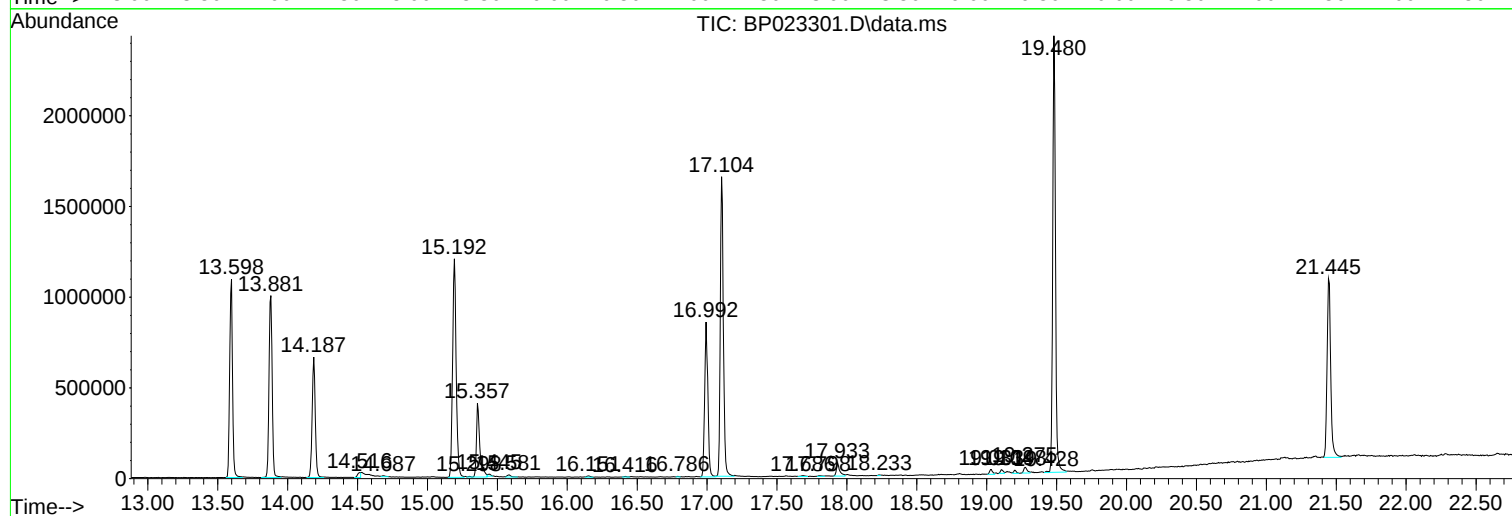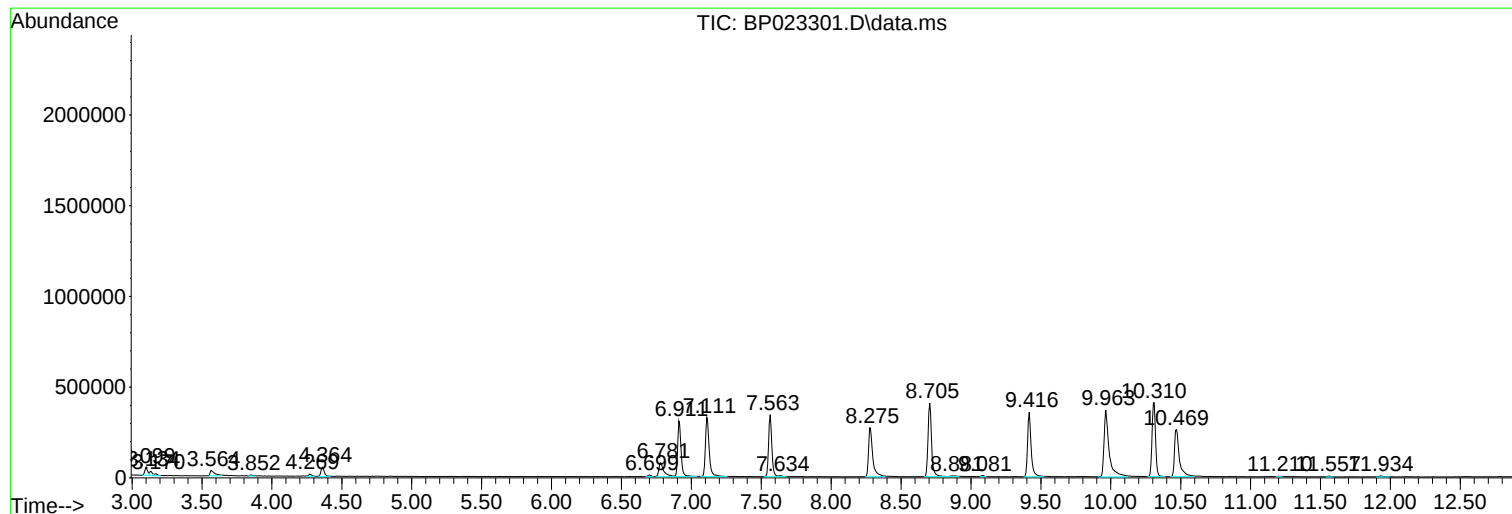

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112224\
Data File : BP023301.D
Acq On : 22 Nov 2024 13:21
Operator : RC/JU
Sample : P4930-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG441

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112224\
Data File : BP023301.D
Acq On : 22 Nov 2024 13:21
Operator : RC/JU
Sample : P4930-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG441

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc