
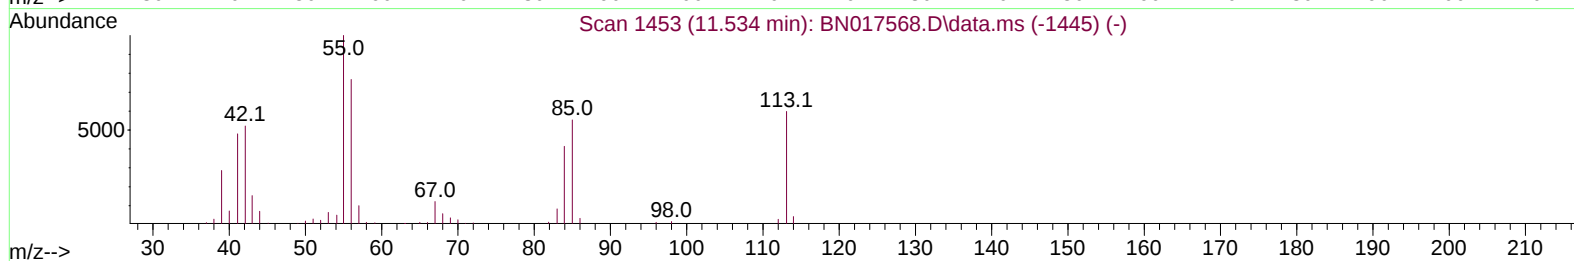
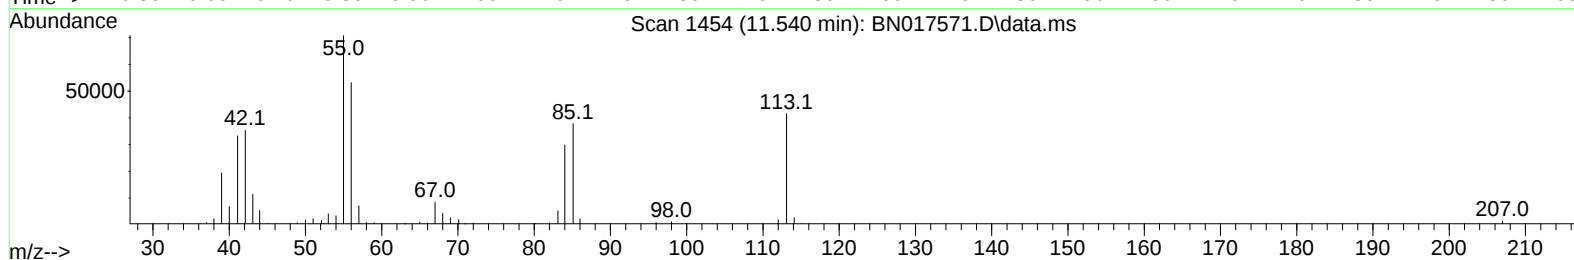


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112421\
Data File : BN017571.D
Acq On : 23 Nov 2021 17:57
Operator : CG/JU
Sample : PB140870BS
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Nov 24 00:58:24 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN112221.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 22 16:16:36 2021
Response via : Initial Calibration

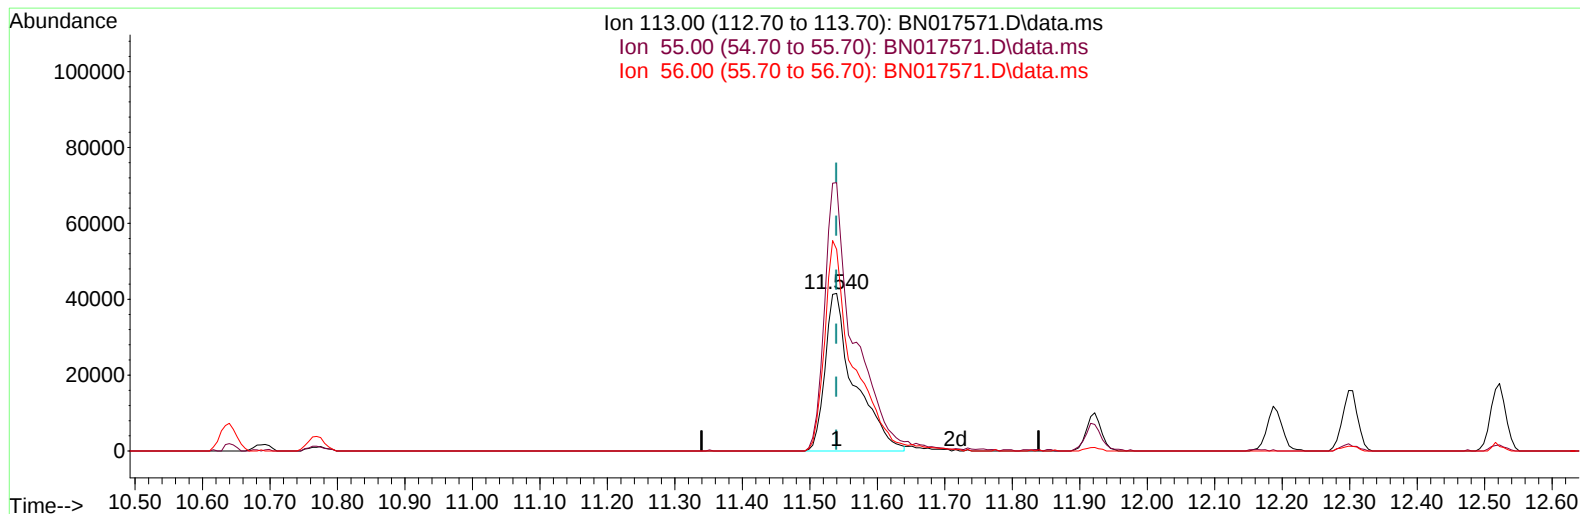

TIC: BN017571.D\data.ms

(34) Caprolactam

11.540min (+ 0.000) 26.85 ng/u1

response 125533

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	176.80	170.33
56.00	129.90	128.01
0.00	0.00	0.00