
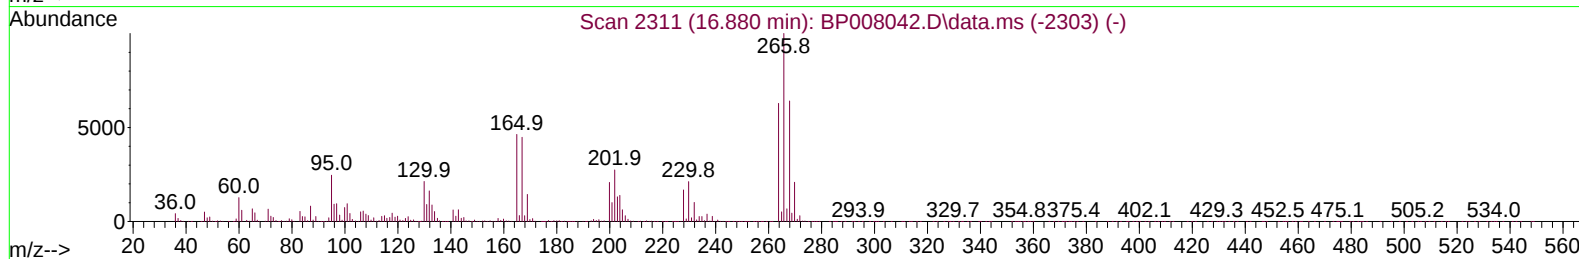
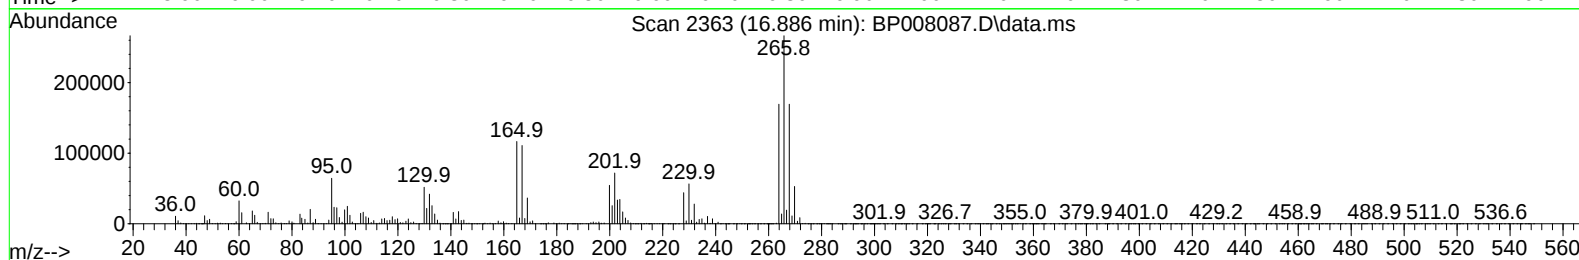


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112321\
Data File : BP008087.D
Acq On : 23 Nov 2021 09:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 23 13:03:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 20 00:21:11 2021
Response via : Initial Calibration

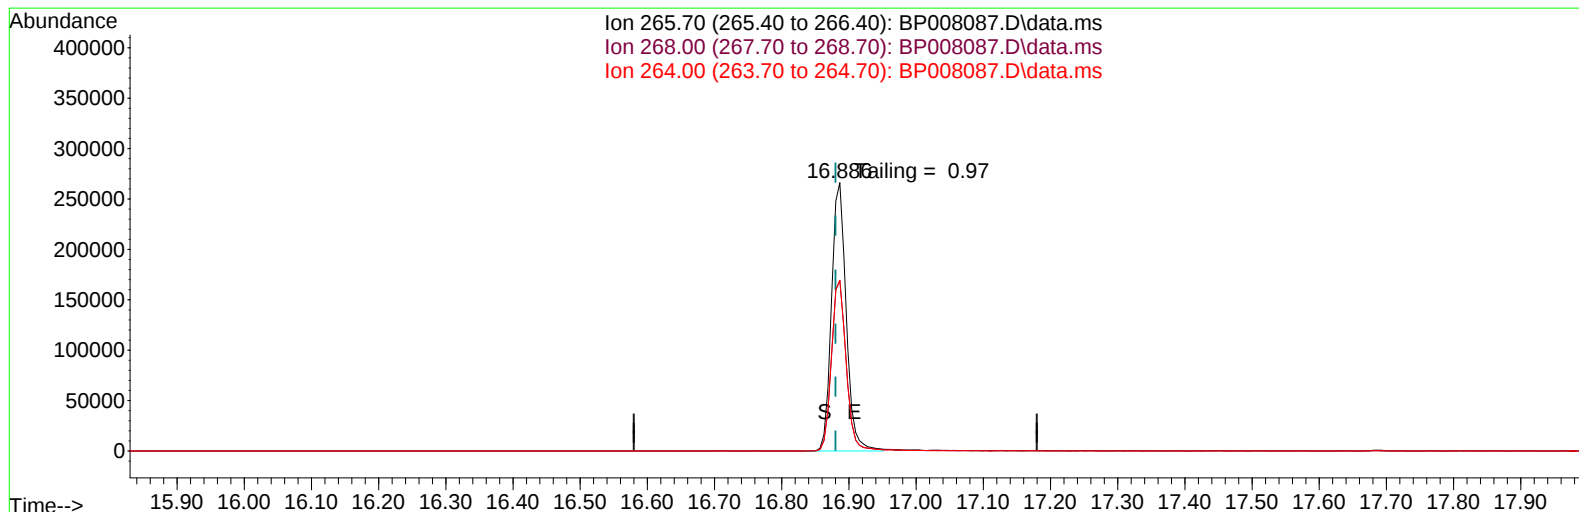

TIC: BP008087.D\data.ms

(70) Pentachlorophenol (C)




16.886min (+ 0.006) 359690.30 ng

response 406746

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	63.61
264.00	62.80	63.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112321\
 Data File : BP008087.D
 Acq On : 23 Nov 2021 09:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 23 13:03:10 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 20 00:21:11 2021
 Response via : Initial Calibration

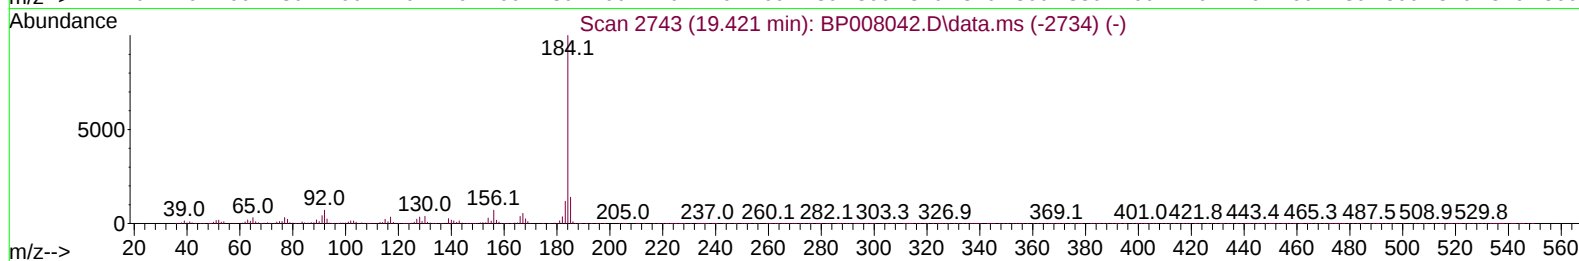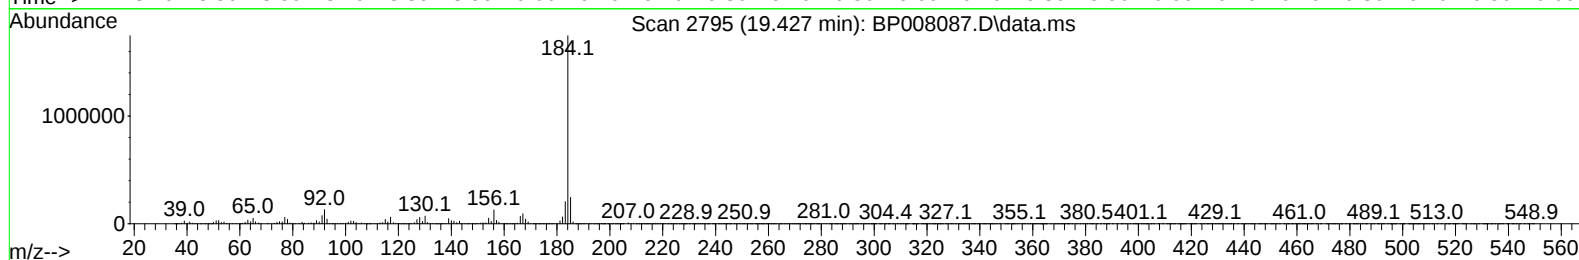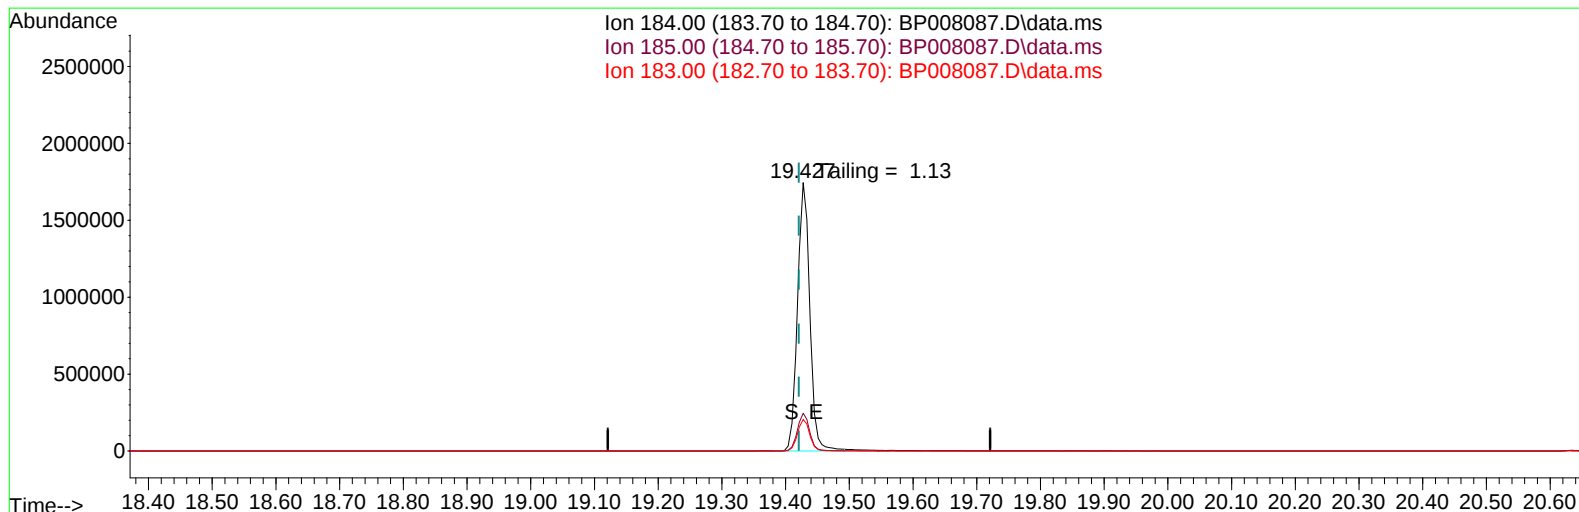

TIC: BP008087.D\data.ms

(77) Benzidine**19.427min (+ 0.006) 11396.11 ng****response 2383605**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.07
183.00	11.80	11.78
0.00	0.00	0.00