
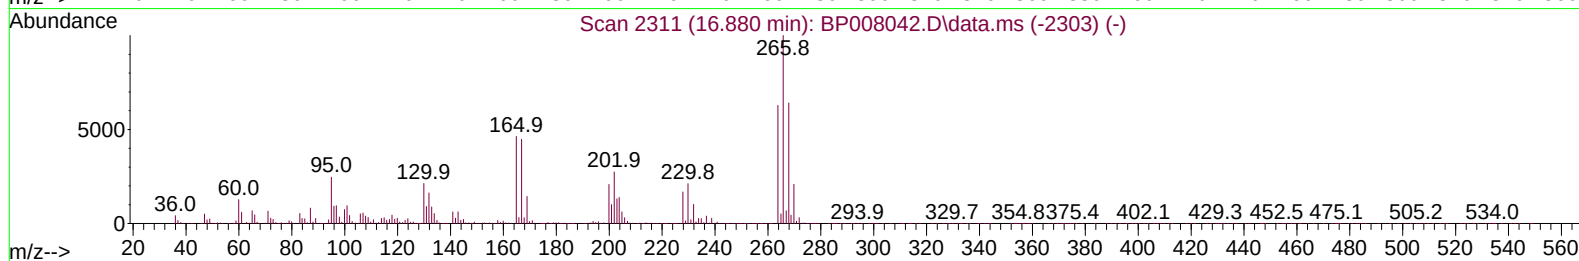
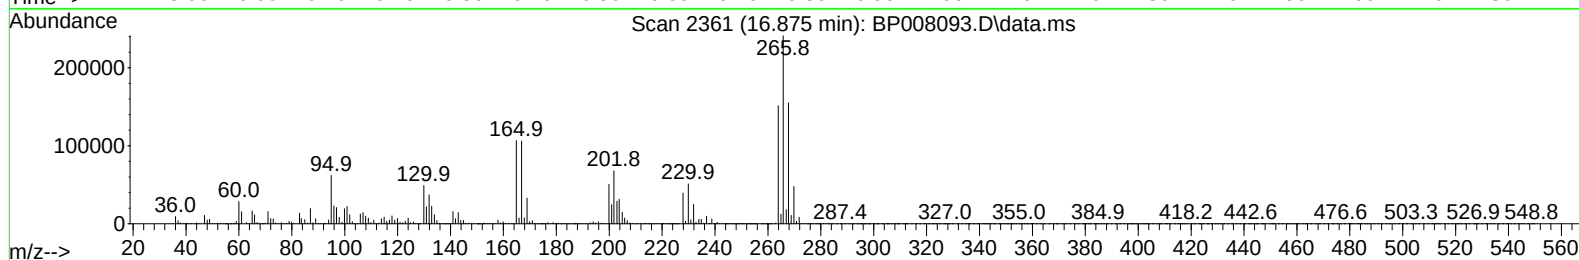


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112321\
 Data File : BP008093.D
 Acq On : 23 Nov 2021 13:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 23 15:40:56 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 20 00:21:11 2021
 Response via : Initial Calibration

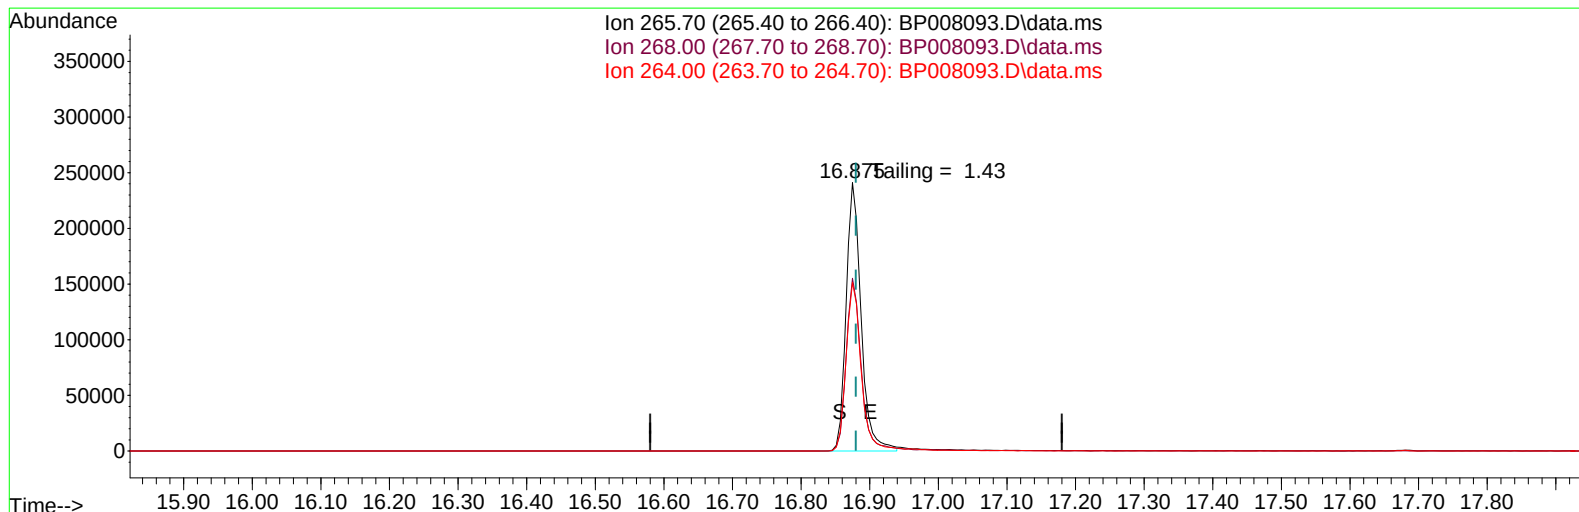

TIC: BP008093.D\data.ms

(70) Pentachlorophenol (C)




16.875min (-0.005) 2549310.46 ng

response 365157

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	64.37
264.00	62.80	62.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112321\
 Data File : BP008093.D
 Acq On : 23 Nov 2021 13:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 23 15:40:56 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 20 00:21:11 2021
 Response via : Initial Calibration

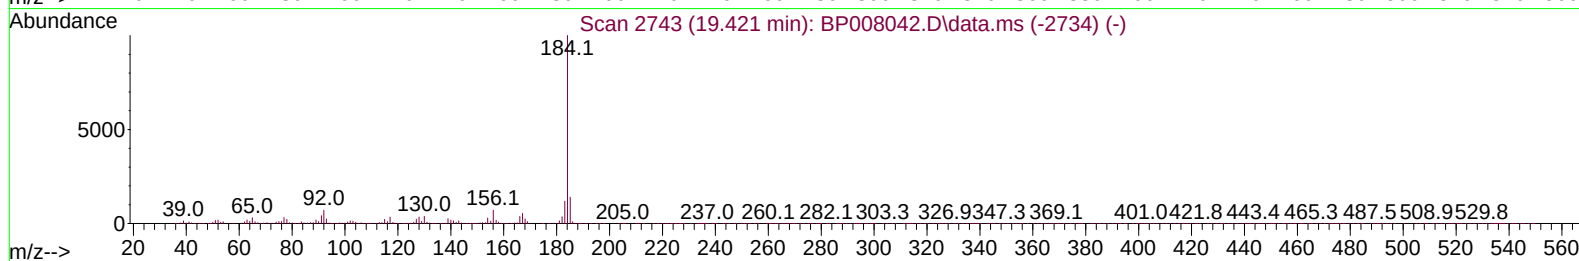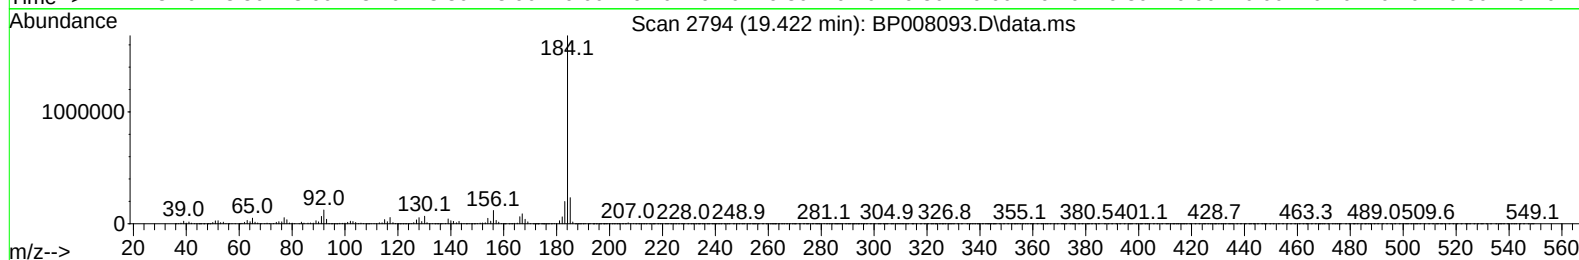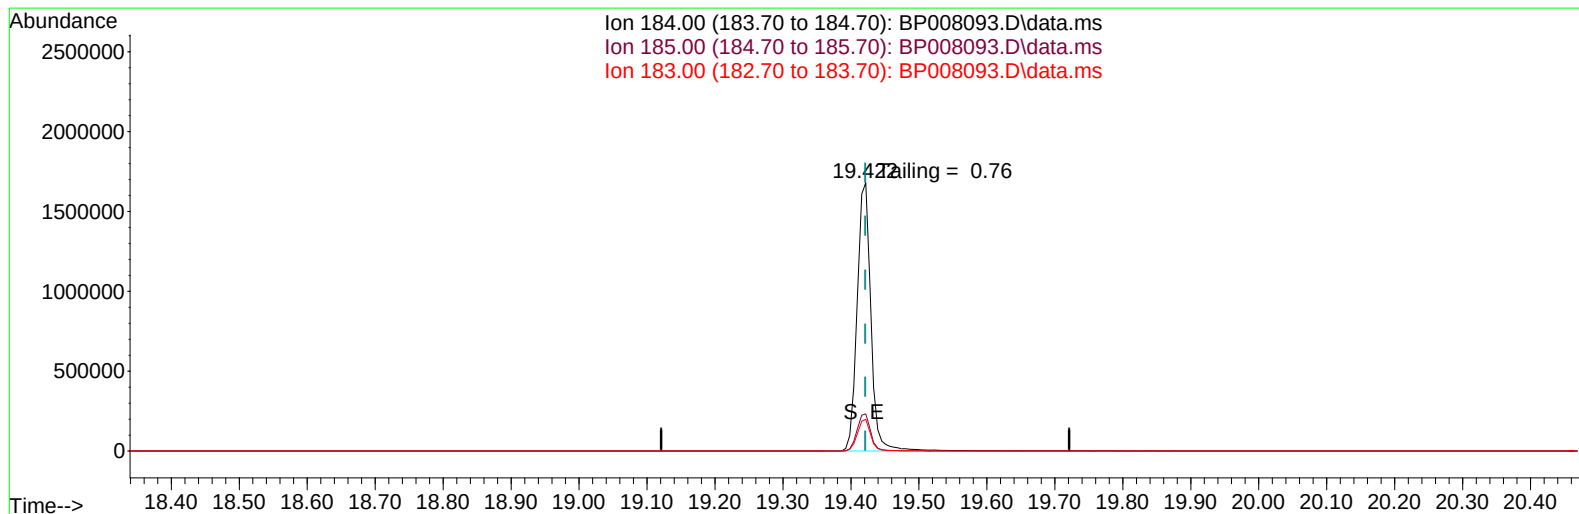

TIC: BP008093.D\data.ms

(77) Benzidine**19.422min (+ 0.001) 2820030.12 ng****response 2258968**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.87
183.00	11.80	11.85
0.00	0.00	0.00