

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112321\
 Data File : BP008095.D
 Acq On : 23 Nov 2021 14:25
 Operator : CG/JU
 Sample : PB140959BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB140959BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008095.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	3	7	17	rVB	112982	137538	1.21%	0.276%
2	5.410	405	412	430	rBV	3176427	4711654	41.45%	9.453%
3	7.004	672	683	696	rBV	2936351	4939873	43.45%	9.910%
4	7.822	813	822	829	rBV	596389	942671	8.29%	1.891%
5	8.981	1010	1019	1037	rBV	1897265	3193485	28.09%	6.407%
6	10.616	1289	1297	1312	rBV	779858	1339792	11.79%	2.688%
7	13.086	1709	1717	1737	rBV	4434636	6923478	60.90%	13.890%
8	14.463	1943	1951	1969	rBV	1326259	1958923	17.23%	3.930%
9	15.957	2198	2205	2226	rBV	3487705	5763545	50.70%	11.563%
10	17.222	2412	2420	2433	rBV	1710723	2616873	23.02%	5.250%
11	19.792	2851	2857	2870	rBV	8362505	11367972	100.00%	22.807%
12	21.321	3111	3117	3126	rBV	2278514	3040407	26.75%	6.100%
13	23.721	3518	3525	3534	rVB2	1390801	2908859	25.59%	5.836%




Sum of corrected areas: 49845070

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112321\
Data File : BP008095.D
Acq On : 23 Nov 2021 14:25
Operator : CG/JU
Sample : PB140959BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140959BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

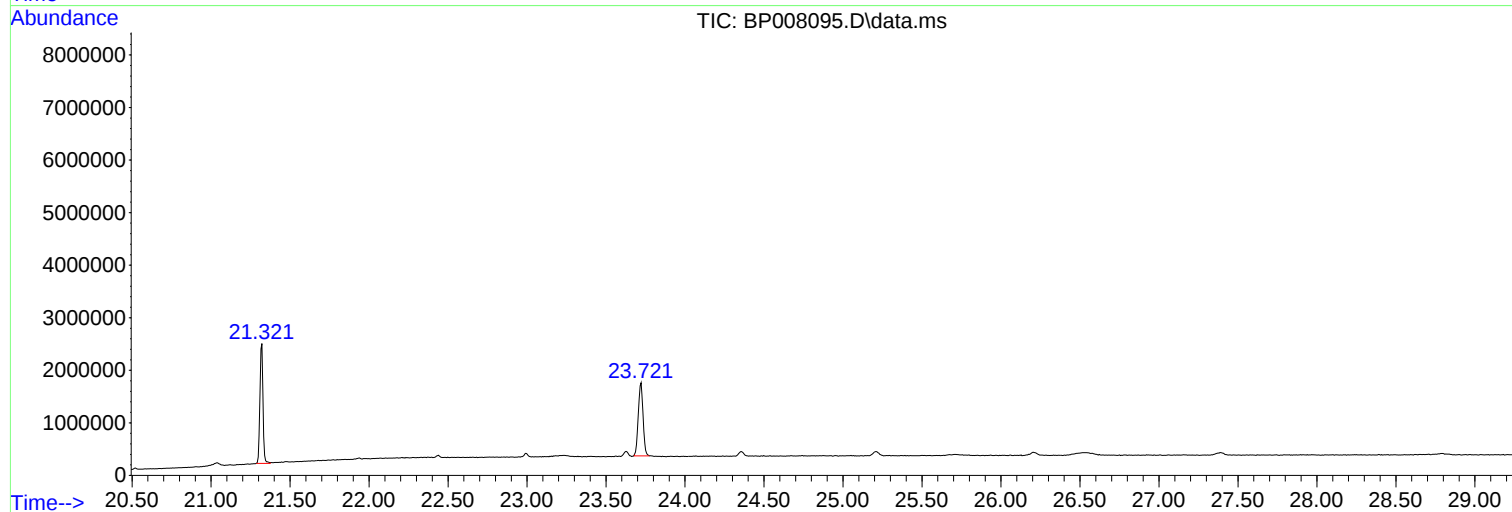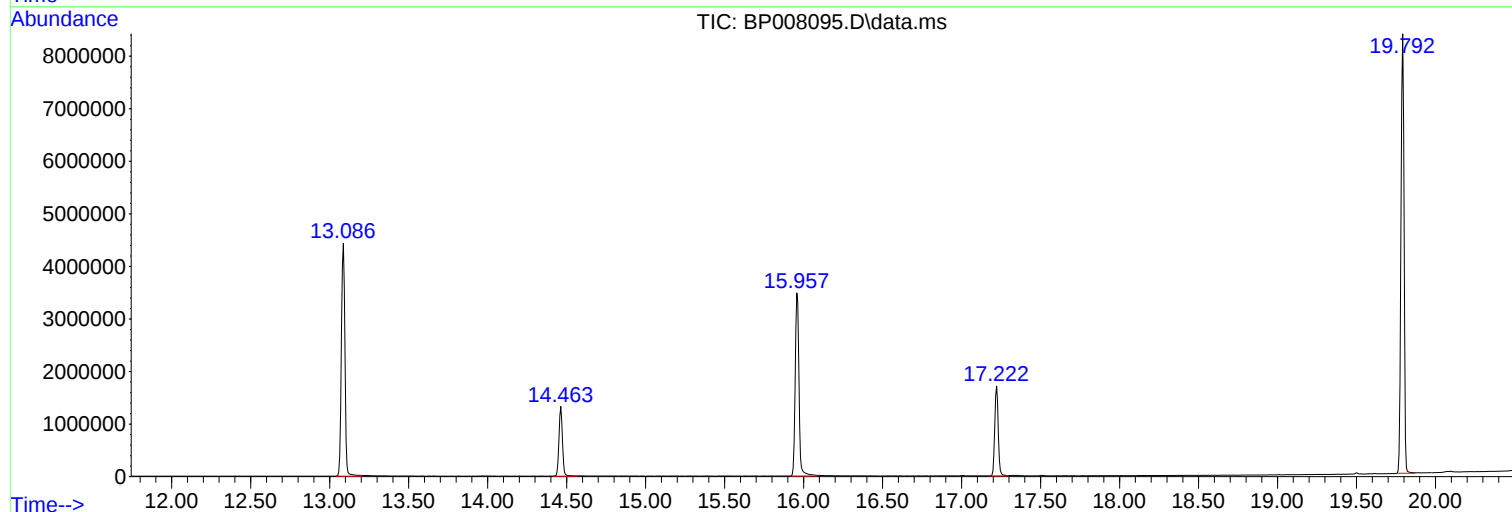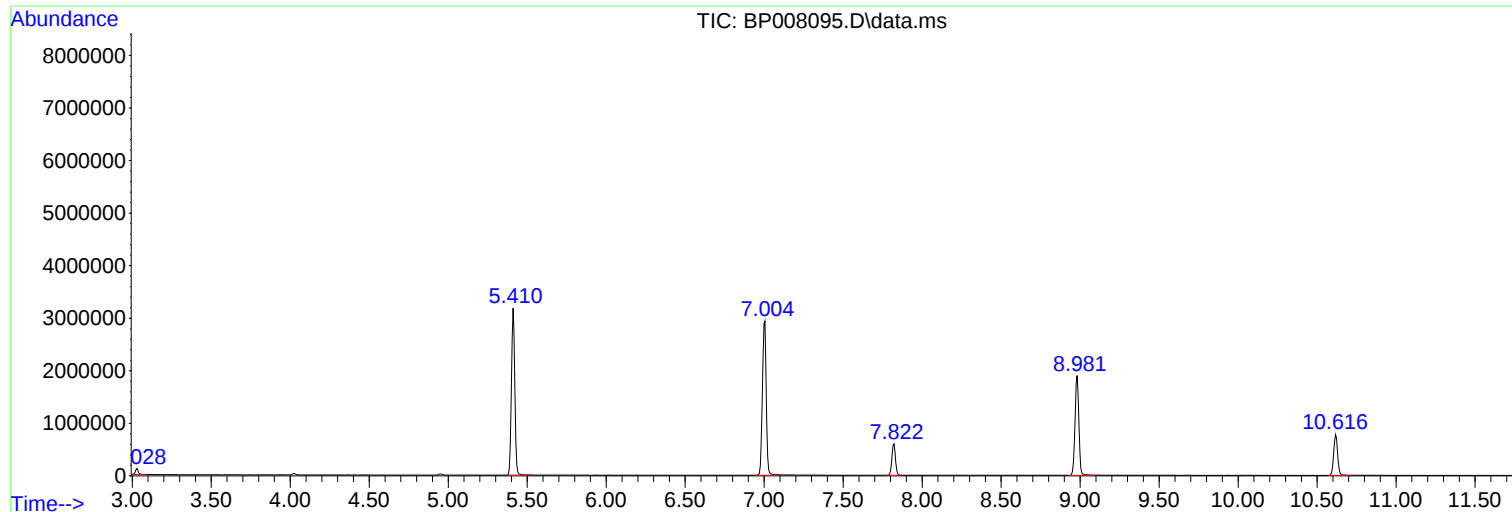

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112321\
Data File : BP008095.D
Acq On : 23 Nov 2021 14:25
Operator : CG/JU
Sample : PB140959BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140959BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.028	2.92 ng	137538	1,4-Dichlorobenzene-d4	7.822

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Silane, tetramethyl-	88	C4H12Si	000075-76-3	25
4			1,3-Dioxolane, 2-propyl-	116	C6H12O2	003390-13-4	17
5			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	9

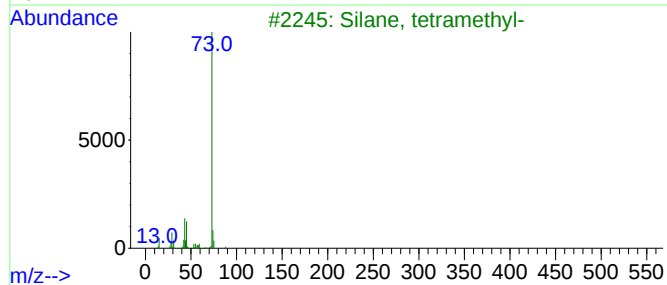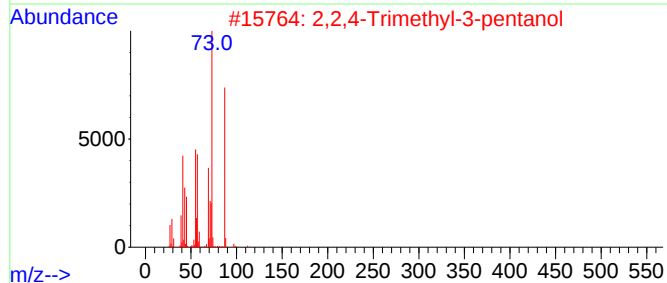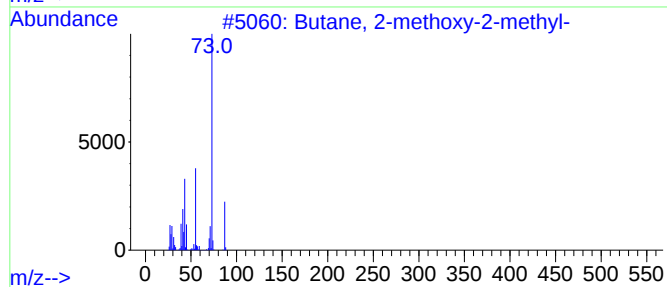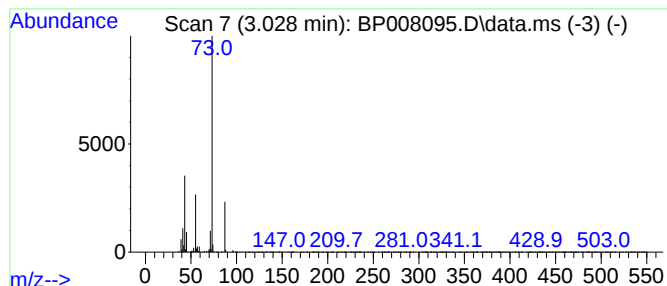

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112321\
Data File : BP008095.D
Acq On : 23 Nov 2021 14:25
Operator : CG/JU
Sample : PB140959BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140959BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.028	2.9	ng	137538	1	7.822	942671	20.0