


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112321\
 Data File : BP008087.D
 Acq On : 23 Nov 2021 09:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 20 00:21:11 2021

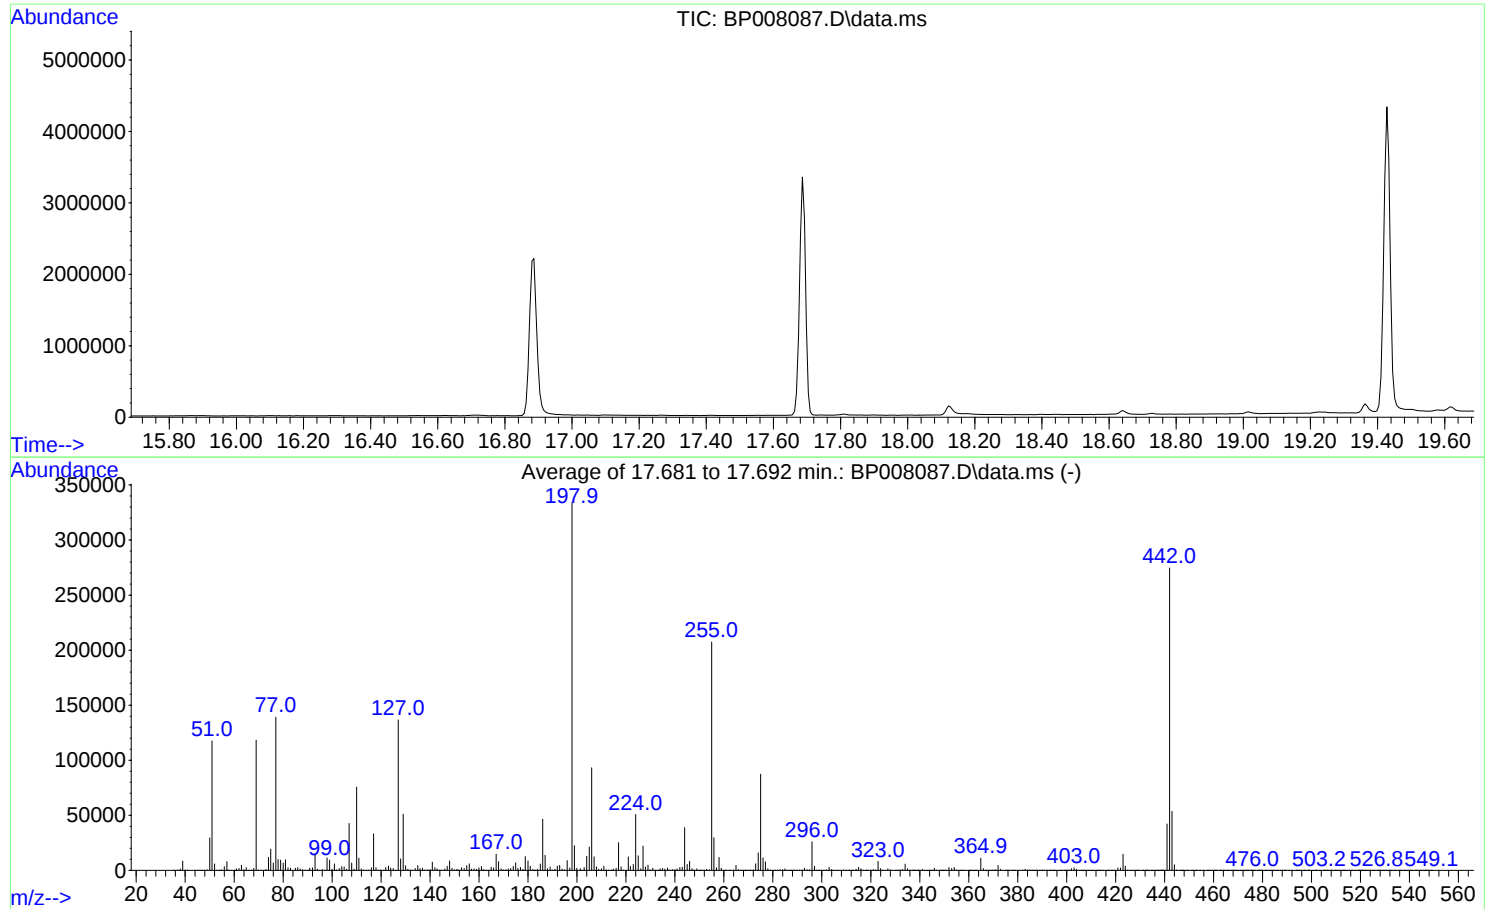




AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	117563	PASS
68	69	0.00	2	1.5	1727	PASS
69	198	0.00	100	35.4	118324	PASS
70	69	0.00	2	0.4	496	PASS
127	198	10	80	40.9	136539	PASS
197	198	0.00	2	0.7	2174	PASS
198	198	100	100	100.0	334073	PASS
199	198	5	9	6.7	22421	PASS
275	198	10	60	26.2	87376	PASS
365	198	1	100	3.3	10981	PASS
441	198	0.01	100	12.6	42200	PASS
442	442	100	100	100.0	274667	PASS
443	442	15	24	19.5	53661	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112321\
Data File : BP008087.D
Acq On : 23 Nov 2021 09:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 23 13:03:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 20 00:21:11 2021
Response via : Initial Calibration

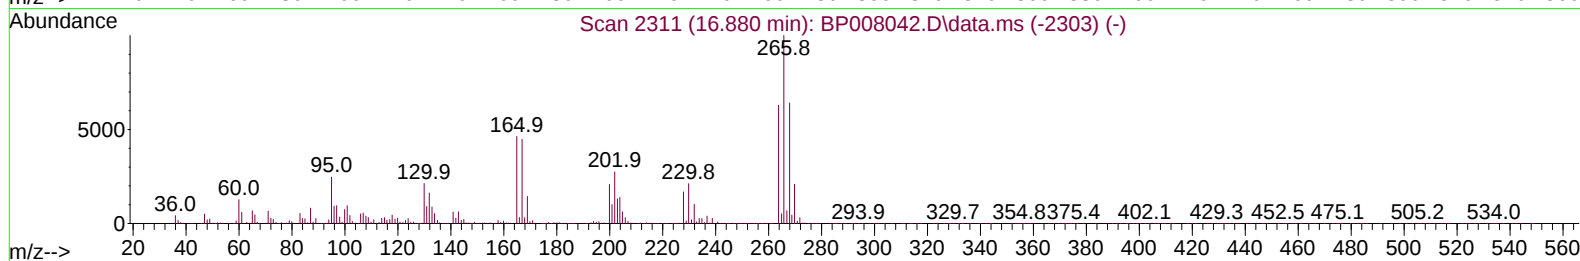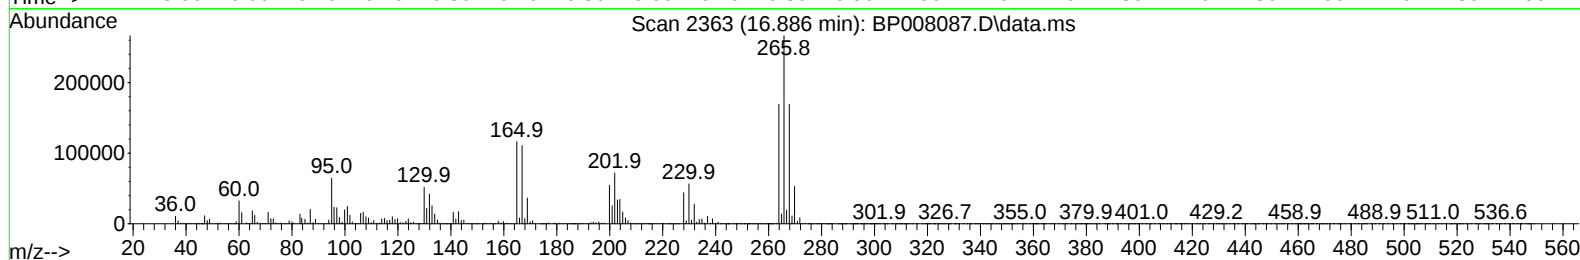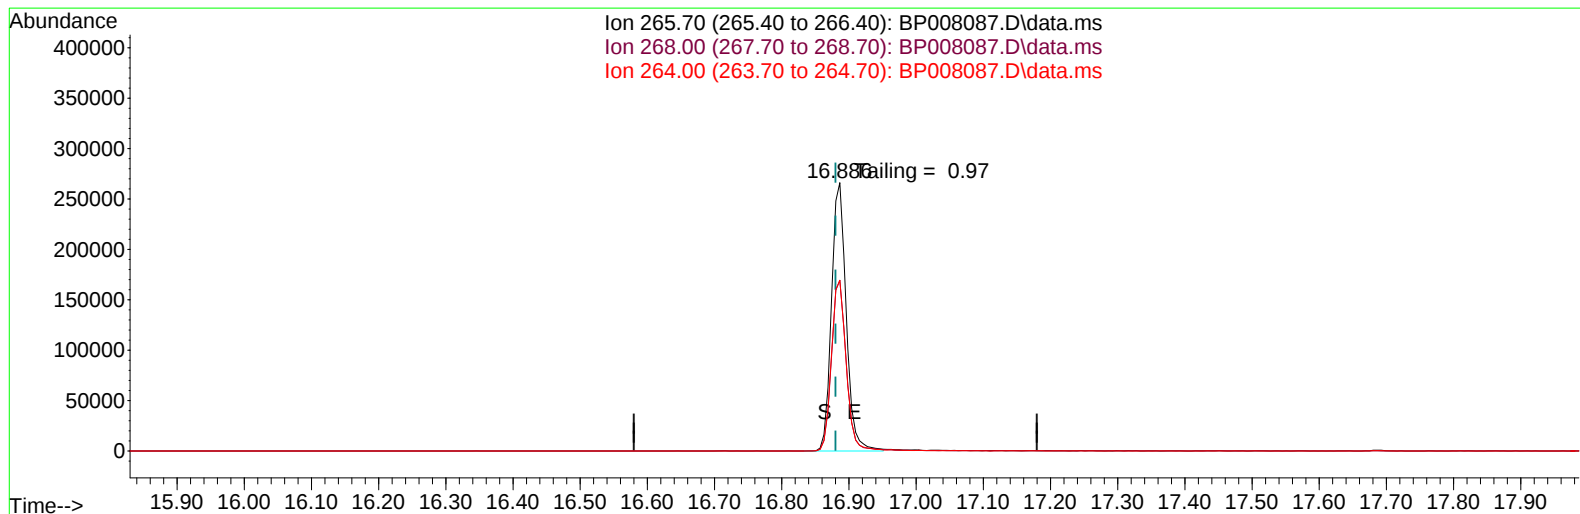

TIC: BP008087.D\data.ms

(70) Pentachlorophenol (C)

16.886min (+ 0.006) 359690.30 ng




response 406746

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	63.61
264.00	62.80	63.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112321\
 Data File : BP008087.D
 Acq On : 23 Nov 2021 09:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 23 13:03:10 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 20 00:21:11 2021
 Response via : Initial Calibration

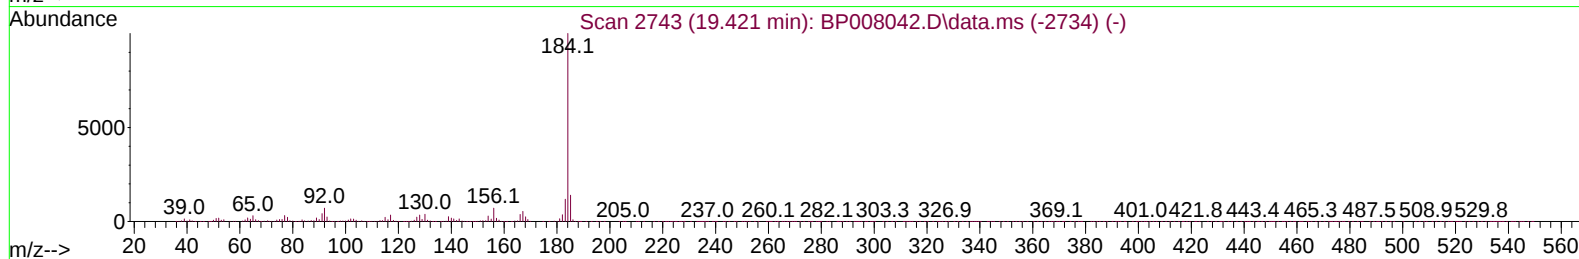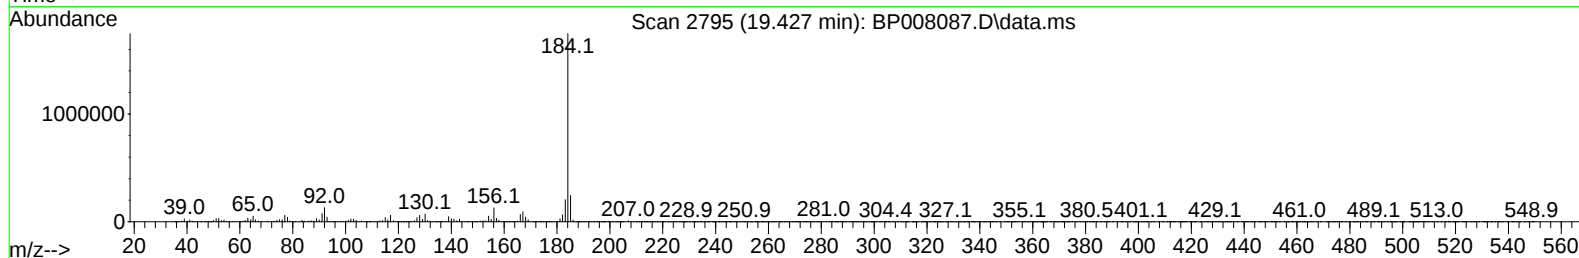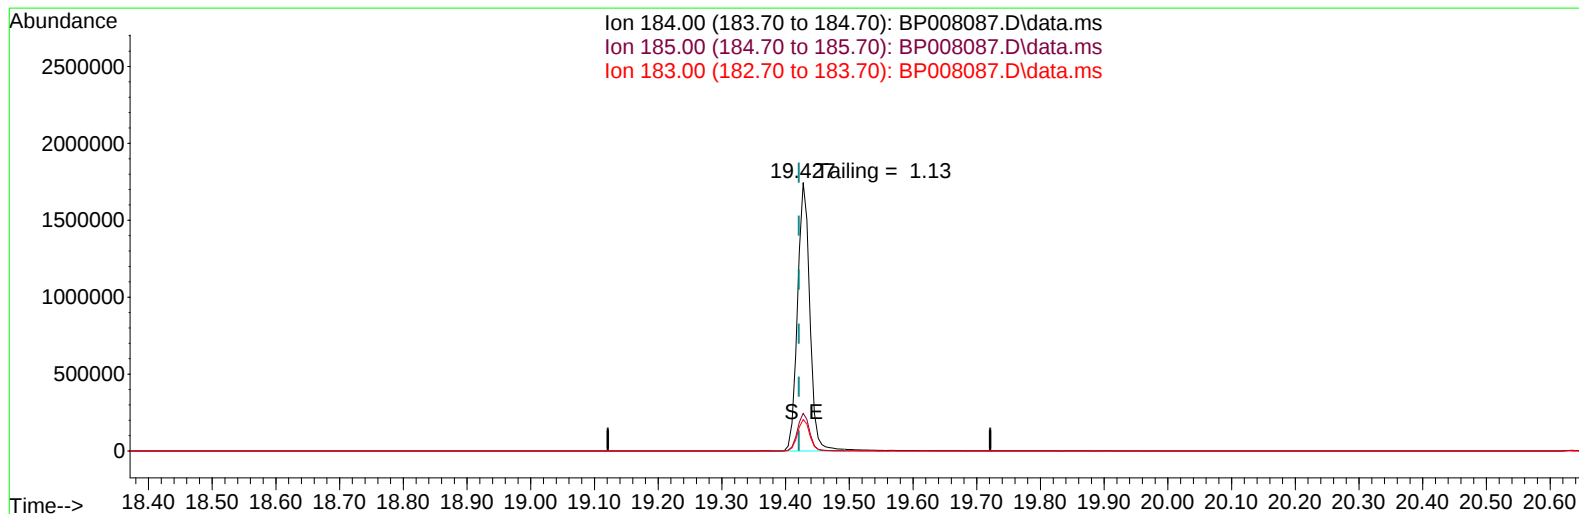

TIC: BP008087.D\data.ms

(77) Benzidine

19.427min (+ 0.006) 11396.11 ng

response 2383605

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.07
183.00	11.80	11.78
0.00	0.00	0.00

Instrument :

BNA_P

ClientSampleId :

DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/23/2021	BNA_P	BP008087.D
Compound Name	Response	Retention Time
DDT	1238797	20.63
DDD	7817	20.2
DDE	1515	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9332	1248129	0.75