


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112321\
 Data File : BP008093.D
 Acq On : 23 Nov 2021 13:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 20 00:21:11 2021

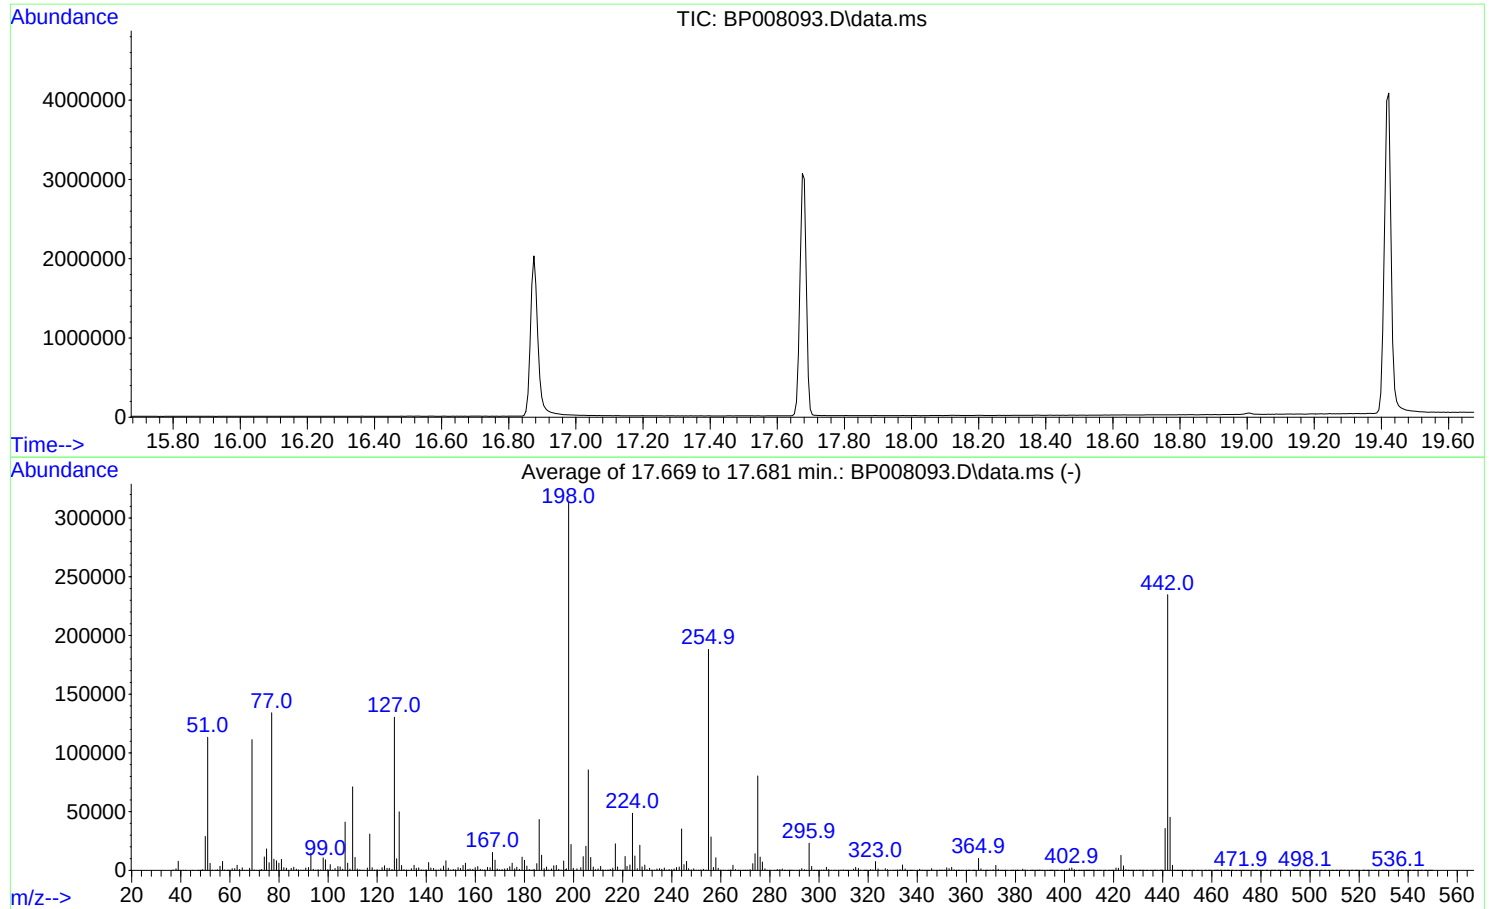




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	113307	PASS
68	69	0.00	2	1.6	1779	PASS
69	198	0.00	100	35.5	111340	PASS
70	69	0.00	2	0.4	492	PASS
127	198	10	80	41.6	130400	PASS
197	198	0.00	2	0.4	1393	PASS
198	198	100	100	100.0	313247	PASS
199	198	5	9	7.1	22128	PASS
275	198	10	60	25.6	80344	PASS
365	198	1	100	3.3	10254	PASS
441	198	0.01	100	11.4	35687	PASS
442	442	100	100	100.0	234752	PASS
443	442	15	24	19.3	45304	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112321\
 Data File : BP008093.D
 Acq On : 23 Nov 2021 13:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 23 15:40:56 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 20 00:21:11 2021
 Response via : Initial Calibration

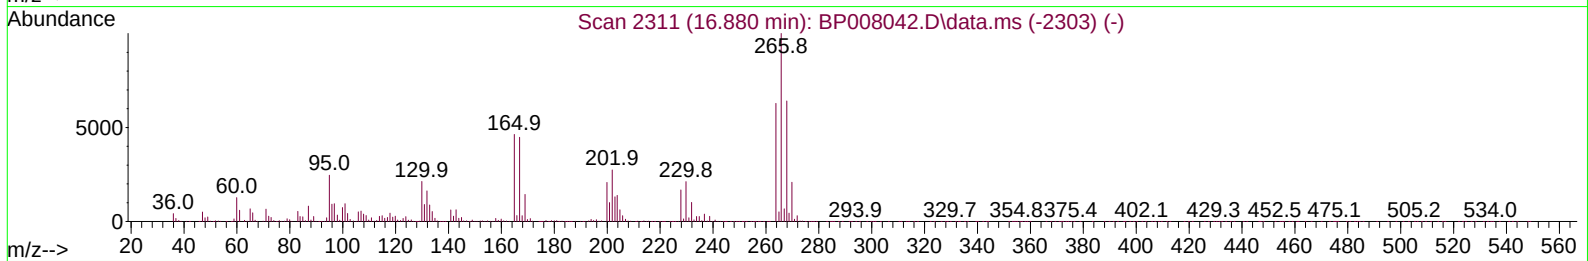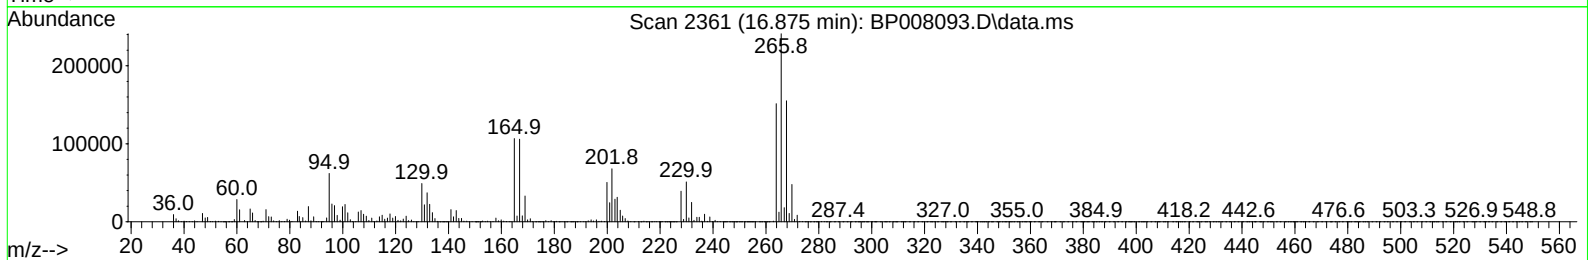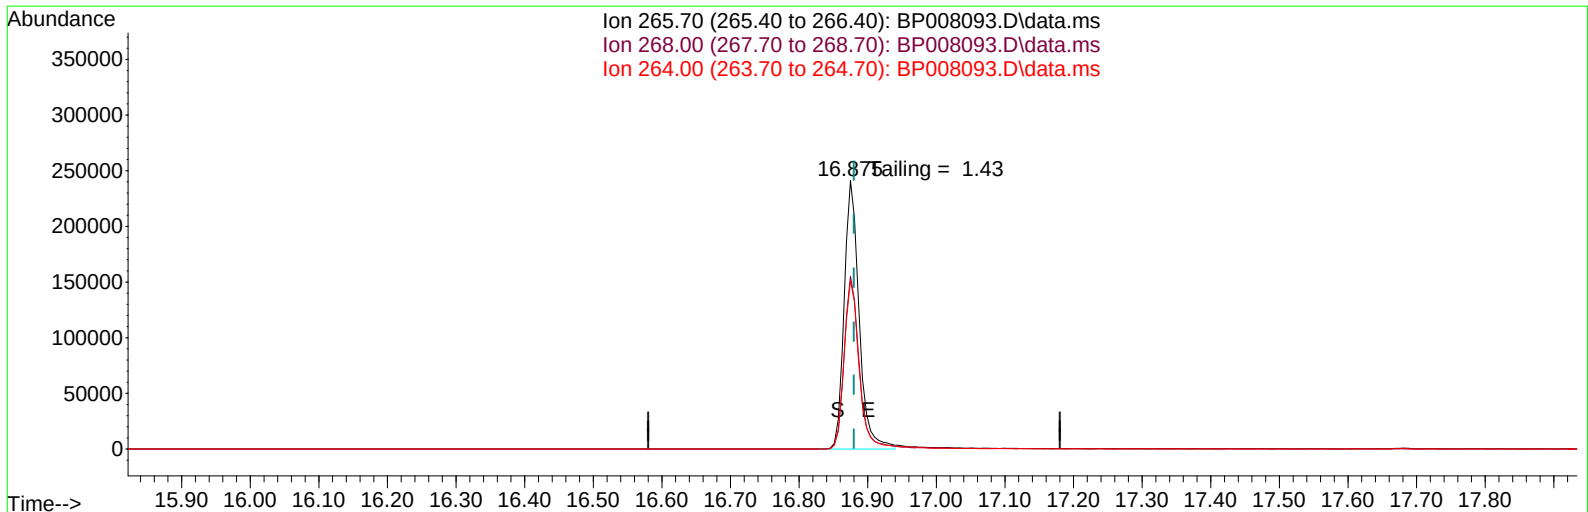

TIC: BP008093.D\data.ms

(70) Pentachlorophenol (C)

16.875min (-0.005) 2549310.46 ng




response 365157

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	64.37
264.00	62.80	62.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112321\
Data File : BP008093.D
Acq On : 23 Nov 2021 13:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 23 15:40:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 20 00:21:11 2021
Response via : Initial Calibration

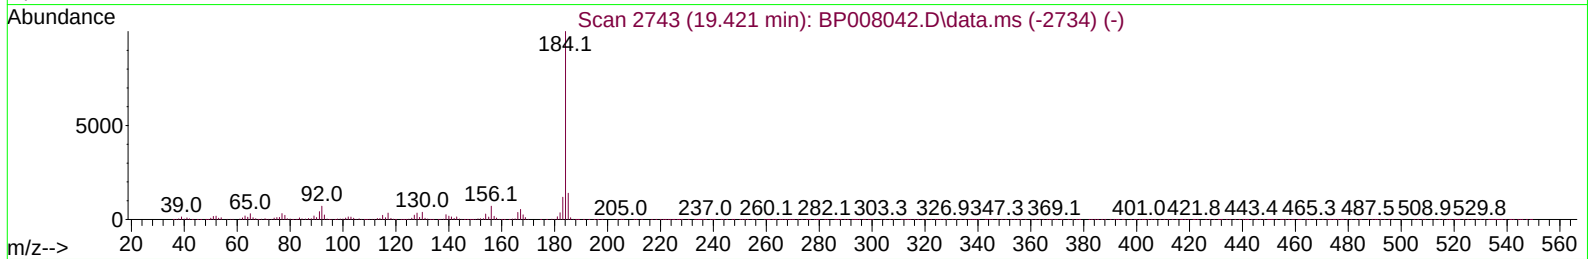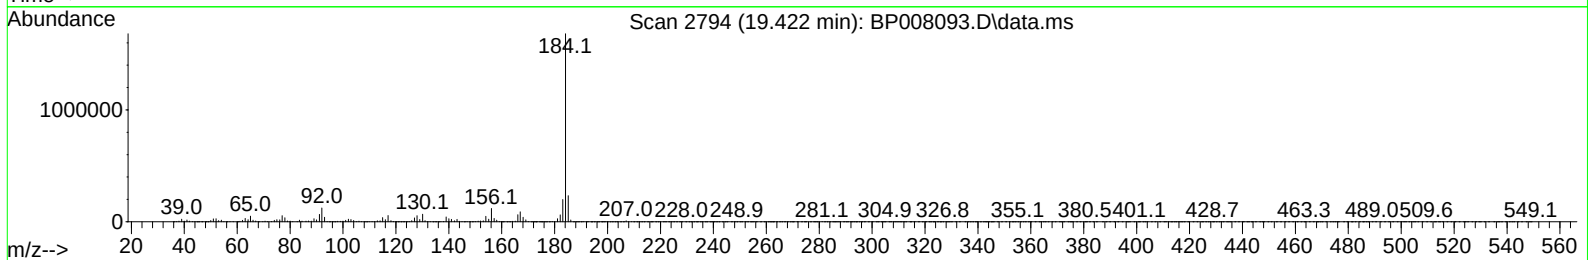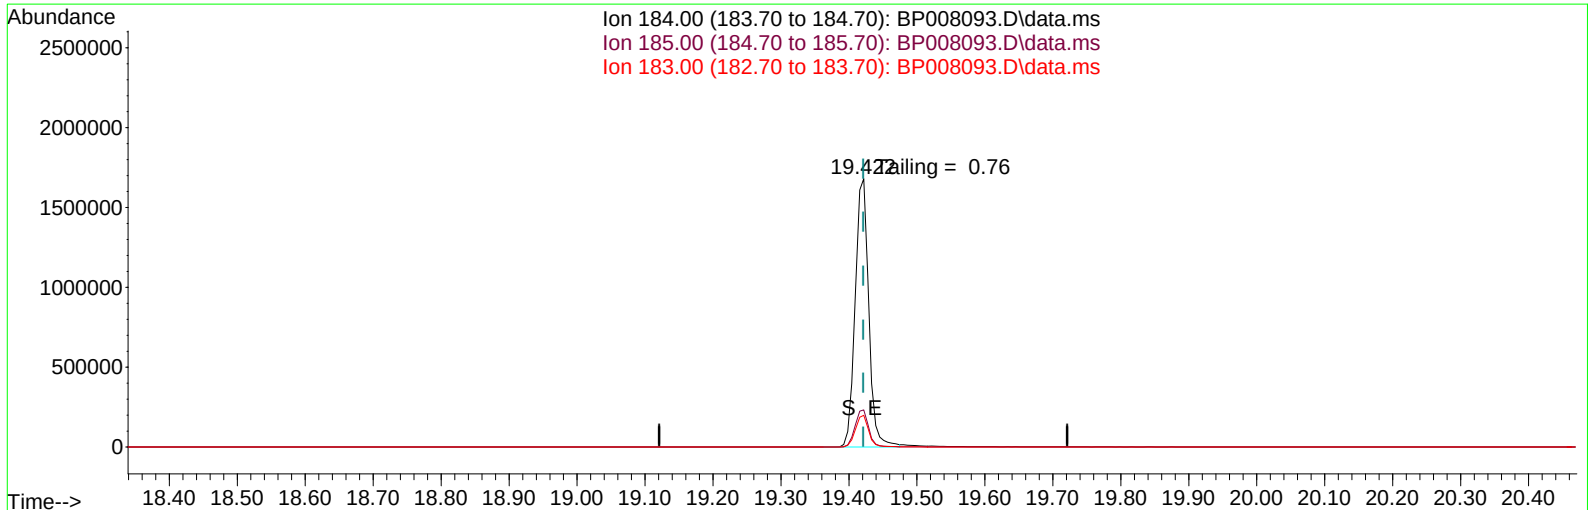

TIC: BP008093.D\data.ms

(77) Benzidine

19.422min (+ 0.001) 2820030.12 ng

response 2258968

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.87
183.00	11.80	11.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/23/2021	BNA_P	<u>BP008093.D</u>
Compound Name	Response	Retention Time
DDT	1185576	20.62
DDD	9143	20.19
DDE	1655	19.7
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10798	1196374	0.90

Instrument :
BNA_P
ClientSampleId :
DFTPP