
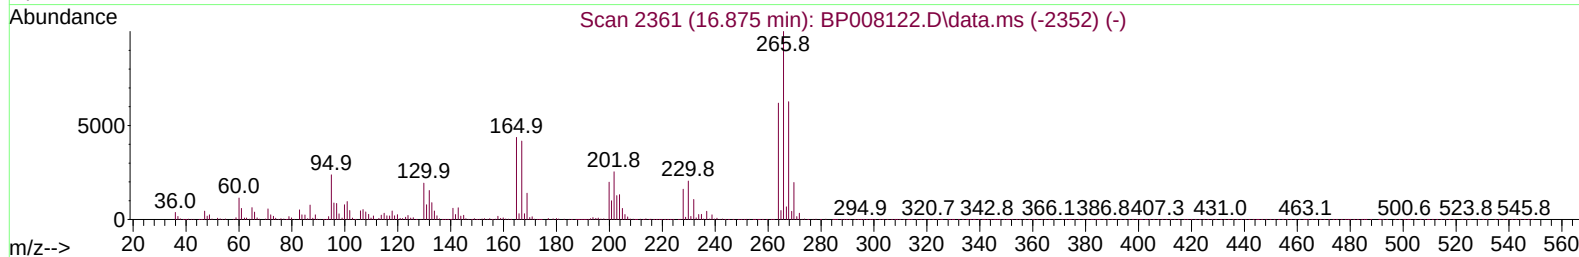
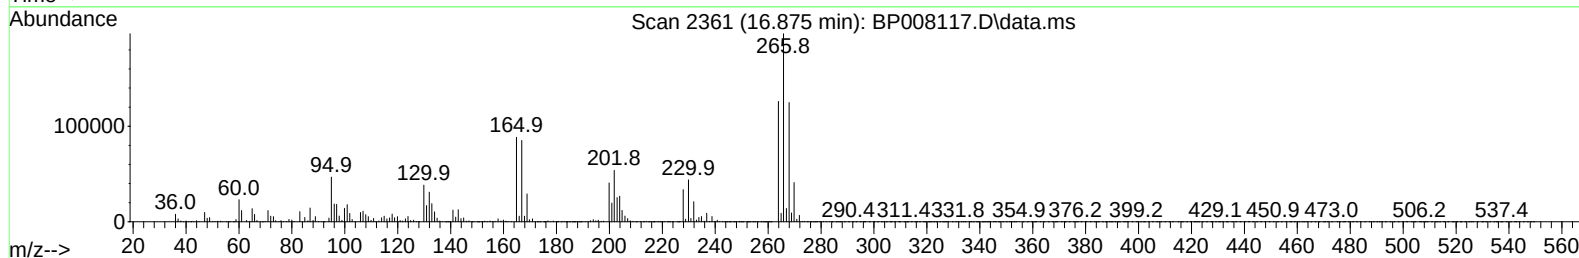


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112521\
 Data File : BP008117.D
 Acq On : 24 Nov 2021 15:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 08:13:04 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 25 01:13:46 2021
 Response via : Initial Calibration

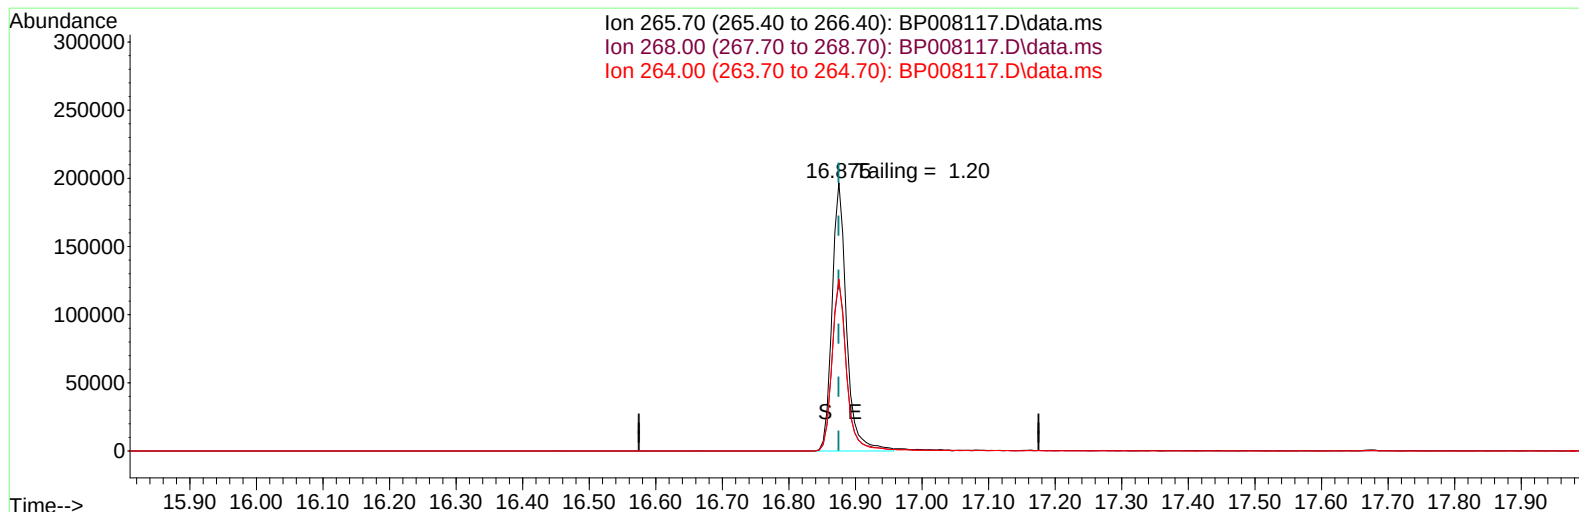

TIC: BP008117.D\data.ms

(70) Pentachlorophenol (C)




16.875min (+ 0.000) 204778.82 ng

response 299610

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.38
264.00	61.90	64.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112521\
 Data File : BP008117.D
 Acq On : 24 Nov 2021 15:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 08:13:04 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 25 01:13:46 2021
 Response via : Initial Calibration

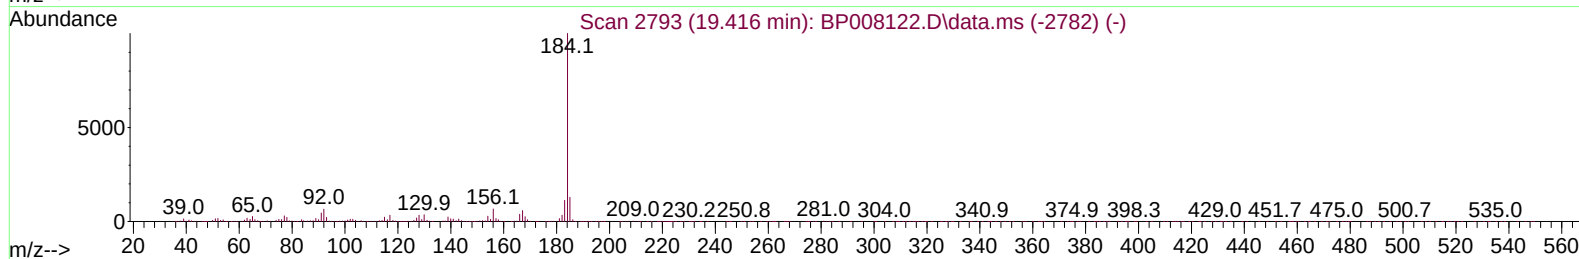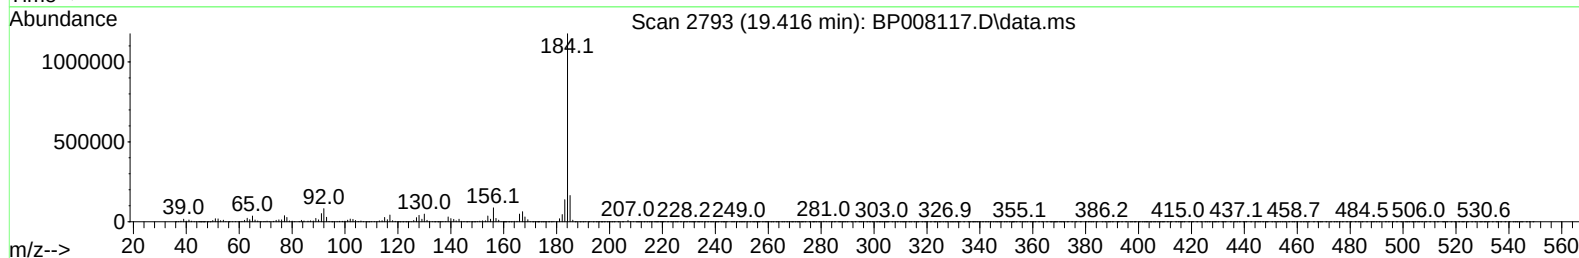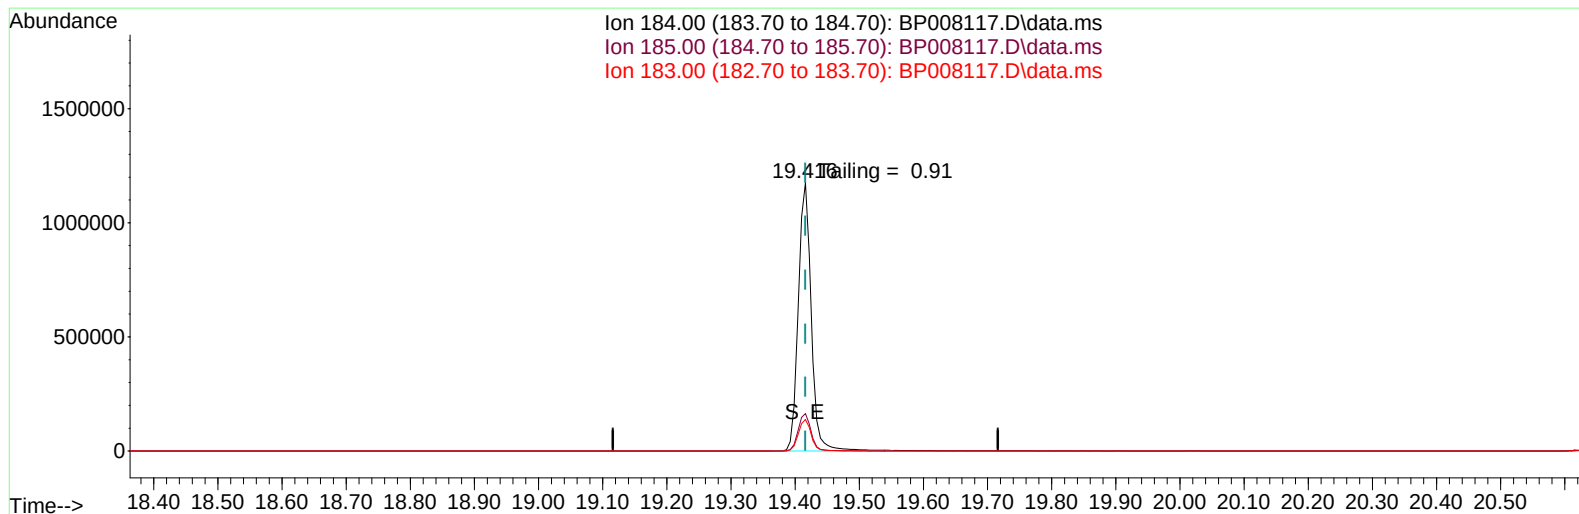

TIC: BP008117.D\data.ms

(77) Benzidine**19.416min (+ 0.000) 179990.55 ng****response 1646803**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.97
183.00	11.40	11.79
0.00	0.00	0.00