
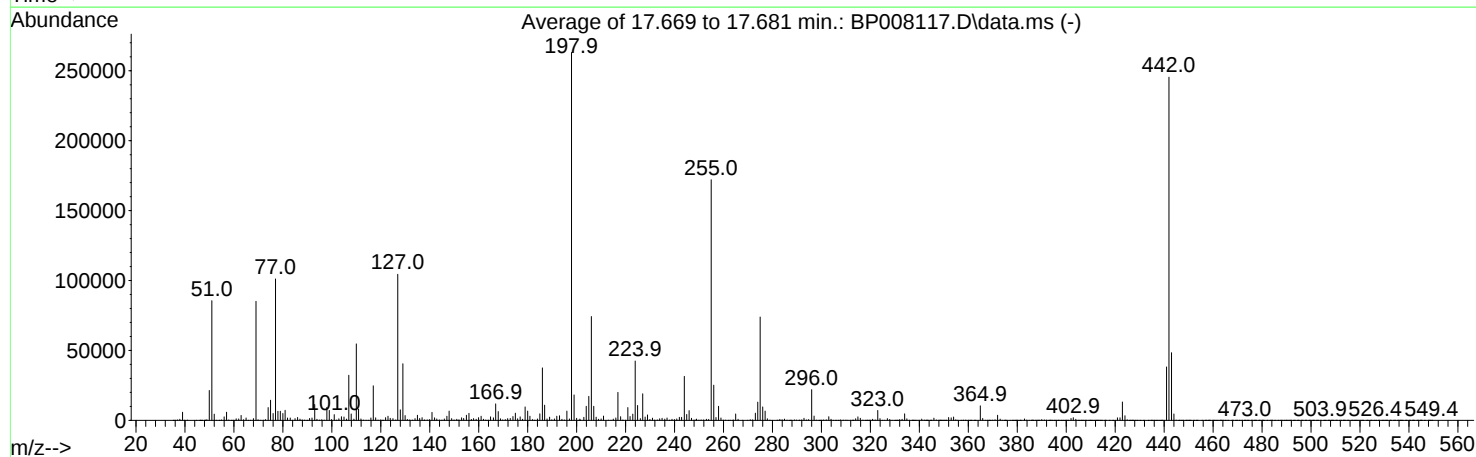


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112521\
 Data File : BP008117.D
 Acq On : 24 Nov 2021 15:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 25 01:13:46 2021

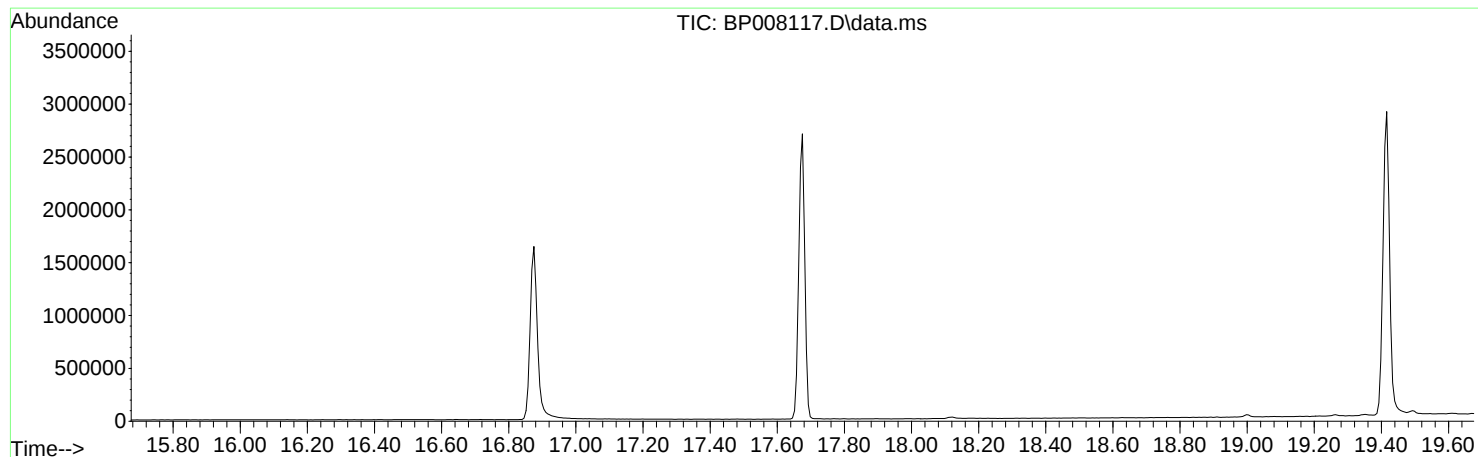

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.5	85580	PASS
68	69	0.00	2	1.5	1319	PASS
69	198	0.00	100	32.3	85097	PASS
70	69	0.00	2	0.5	440	PASS
127	198	10	80	39.7	104455	PASS
197	198	0.00	2	0.4	1023	PASS
198	198	100	100	100.0	263070	PASS
199	198	5	9	6.9	18168	PASS
275	198	10	60	28.1	73872	PASS
365	198	1	100	4.0	10412	PASS
441	198	0.01	100	14.6	38277	PASS
442	442	100	100	100.0	245486	PASS
443	442	15	24	19.7	48371	PASS

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP


DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/25/2021	BNA_P	<u>BP008117.D</u>
Compound Name	Response	Retention Time
DDT	864071	20.622
DDD	15997	20.192
DDE	1126	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17123	881194	1.94

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112521\
Data File : BP008117.D
Acq On : 24 Nov 2021 15:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 25 08:13:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 25 01:13:46 2021
Response via : Initial Calibration

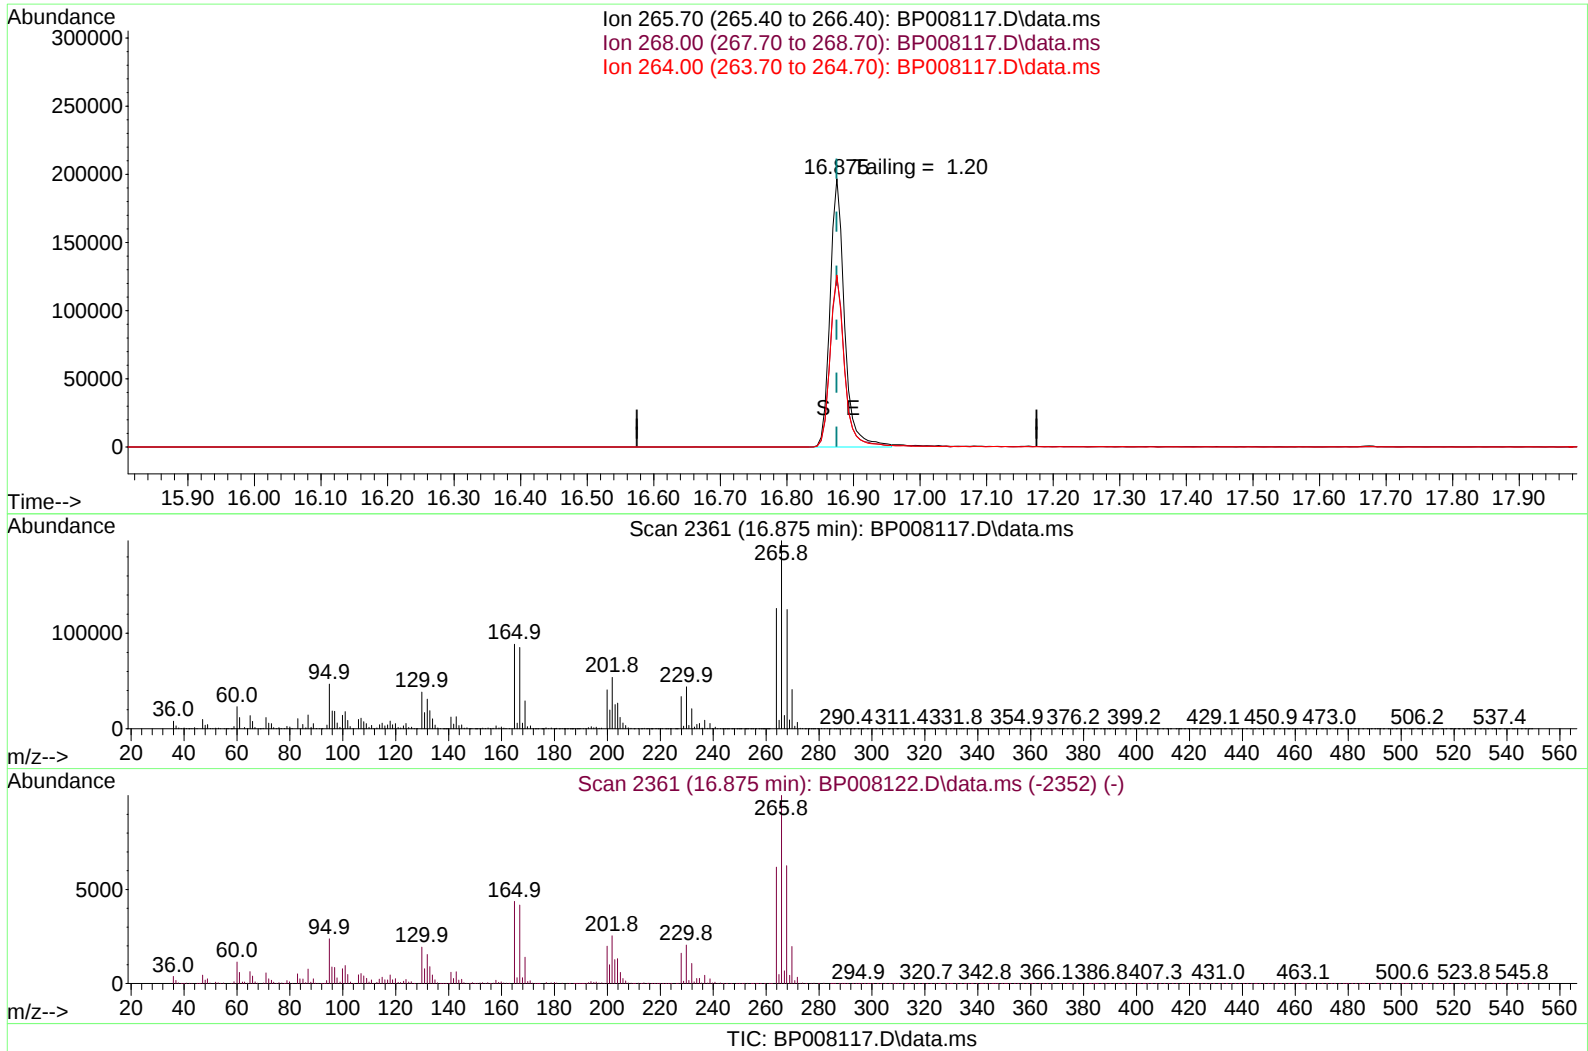

(70) Pentachlorophenol (C)

16.875min (+ 0.000) 204778.82 ng




response 299610

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.38
264.00	61.90	64.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112521\
 Data File : BP008117.D
 Acq On : 24 Nov 2021 15:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 25 08:13:04 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 25 01:13:46 2021
 Response via : Initial Calibration

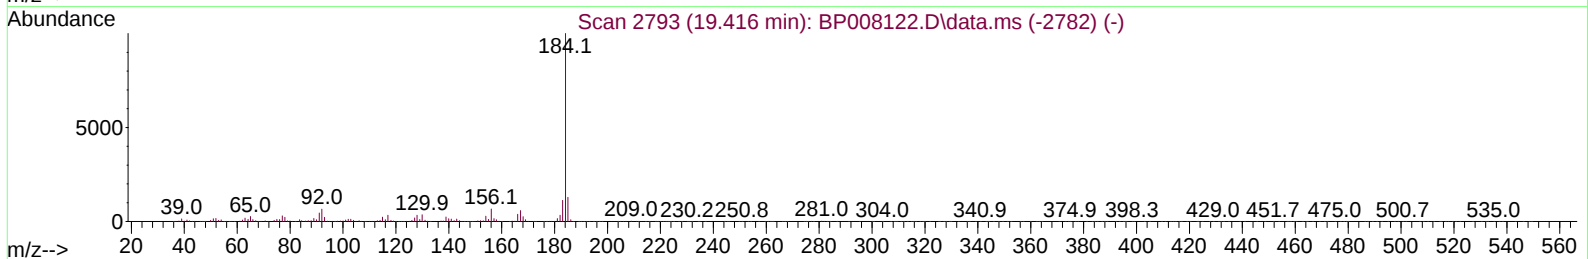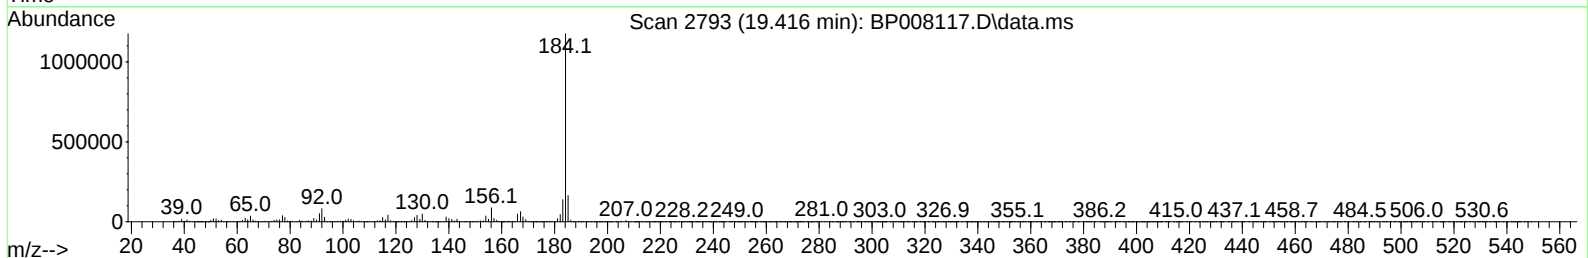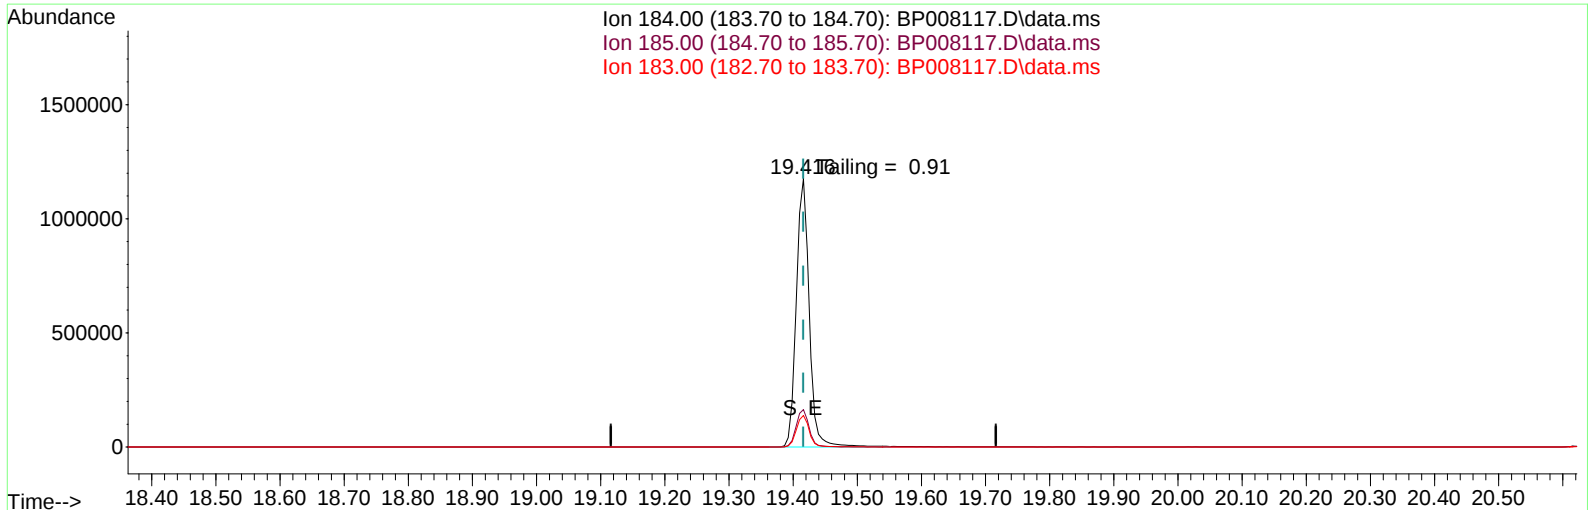

TIC: BP008117.D\data.ms

(77) Benzidine

19.416min (+ 0.000) 179990.55 ng

response 1646803

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.97
183.00	11.40	11.79
0.00	0.00	0.00