

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012781.D
 Acq On : 26 Nov 2022 23:16
 Operator : CG/JU
 Sample : N5694-08
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB44

Quant Time: Nov 27 23:01:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	487938	20.000	ng/u1	0.00
20) Naphthalene-d8	10.834	136	2189251	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.651	164	1463551	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.410	188	3238041	20.000	ng/u1	0.00
79) Chrysene-d12	21.492	240	3273564	20.000	ng/u1	0.00
88) Perylene-d12	24.010	264	3403114	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	60403	5.305	ng/uL	0.00
4) Pyridine-d5	3.822	84	252001	7.395	ng/u1	0.00
7) Phenol-d5	7.163	99	289203	7.213	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	852491	34.505	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	822650	26.926	ng/u1	0.00
15) 4-Methylphenol-d8	8.716	113	550184	17.031	ng/u1	0.00
21) Nitrobenzene-d5	9.181	128	513996	38.359	ng/u1	0.00
24) 2-Nitrophenol-d4	9.910	143	531914	37.386	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.446	165	993213	29.919	ng/u1	0.00
31) 4-Chloroaniline-d4	10.963	131	1137339	25.019	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	3755197	37.277	ng/u1	0.00
49) Acenaphthylene-d8	14.345	160	4244723	36.112	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	86464	4.814	ng/u1	0.00
60) Fluorene-d10	15.645	176	3330792	37.754	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	433992	28.043	ng/u1	0.00
73) Anthracene-d10	17.510	188	5408198	37.943	ng/u1	0.00
81) Pyrene-d10	19.733	212	6439998	33.857	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.851	264	6356532	38.027	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.434	88	146113	11.948	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012781.D
Acq On : 26 Nov 2022 23:16
Operator : CG/JU
Sample : N5694-08
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB44

Quant Time: Nov 27 23:01:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration

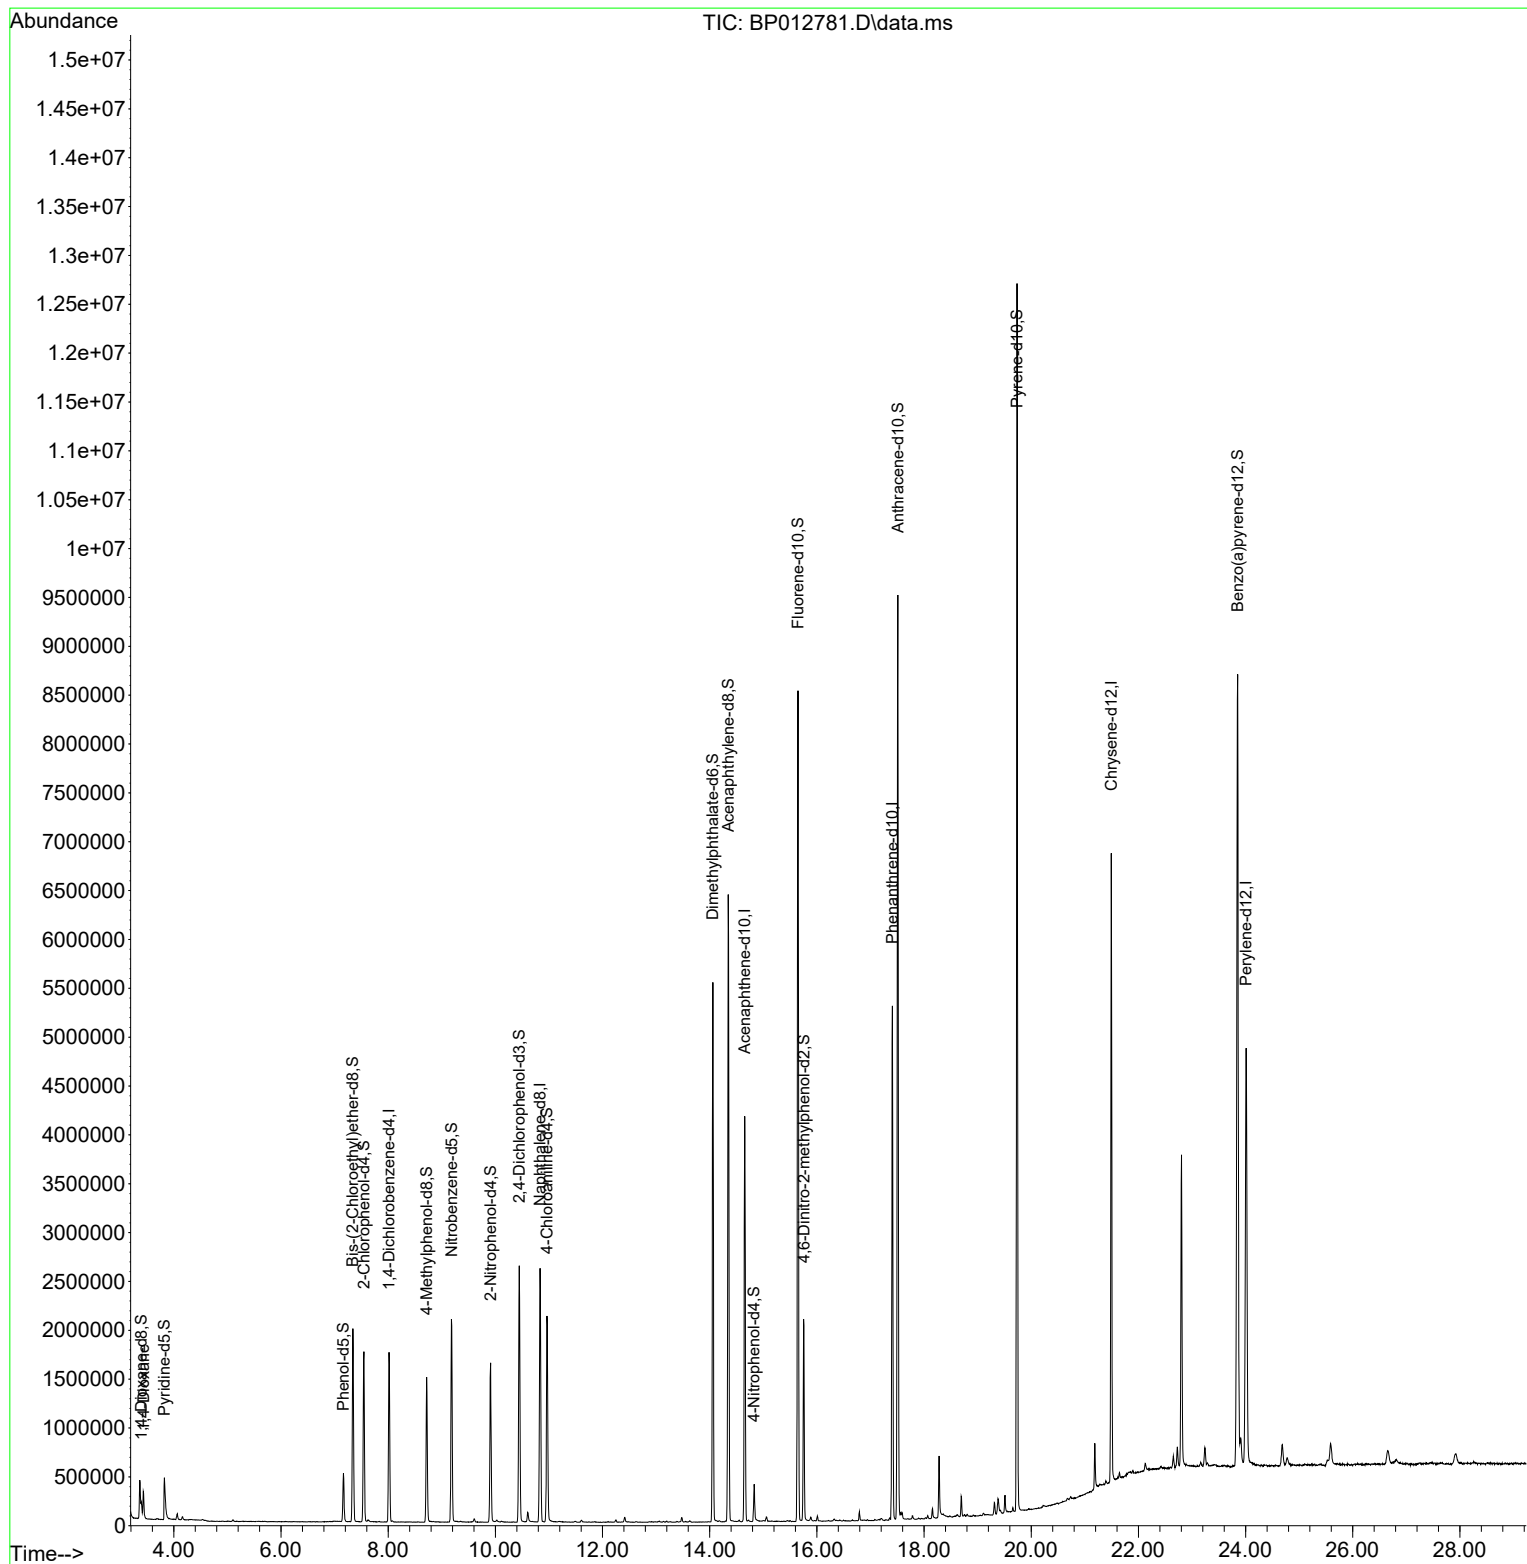

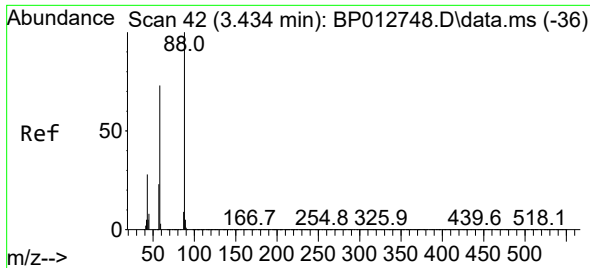

#2
 1,4-Dioxane
 Concen: 11.948 ng/uL
 RT: 3.434 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BP012781.D
 Acq: 26 Nov 2022 23:16

Instrument :
 BNA_P
 ClientSampleId :
 BHB44

Tgt Ion: 88 Resp: 146113
 Ion Ratio Lower Upper
 88 100
 43 28.1 22.6 34.0
 58 70.4 59.6 89.4

