

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP112522\  
 Data File : BP012785.D  
 Acq On : 27 Nov 2022 01:32  
 Operator : CG/JU  
 Sample : N5710-04  
 Misc :  
 ALS Vial : 59 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 C0KY3

Quant Time: Nov 27 23:02:11 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP112522.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Sun Nov 27 22:55:08 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|-------------------------------|--------|------|----------|--------|-------|----------|
| Internal Standards            |        |      |          |        |       |          |
| 1) 1,4-Dichlorobenzene-d4     | 8.017  | 152  | 533897   | 20.000 | ng/u1 | 0.00     |
| 20) Naphthalene-d8            | 10.834 | 136  | 2417737  | 20.000 | ng/u1 | 0.00     |
| 38) Acenaphthene-d10          | 14.651 | 164  | 1650780  | 20.000 | ng/u1 | 0.00     |
| 64) Phenanthrene-d10          | 17.410 | 188  | 3670005  | 20.000 | ng/u1 | 0.00     |
| 79) Chrysene-d12              | 21.492 | 240  | 3632852  | 20.000 | ng/u1 | 0.00     |
| 88) Perylene-d12              | 24.010 | 264  | 3625304  | 20.000 | ng/u1 | 0.00     |
| System Monitoring Compounds   |        |      |          |        |       |          |
| 3) 1,4-Dioxane-d8             | 3.393  | 96   | 58030    | 4.658  | ng/uL | 0.00     |
| 4) Pyridine-d5                | 3.823  | 84   | 261763   | 7.020  | ng/u1 | 0.00     |
| 7) Phenol-d5                  | 7.164  | 99   | 235074   | 5.358  | ng/u1 | 0.00     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.340  | 67   | 802654   | 29.691 | ng/u1 | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.546  | 132  | 741350   | 22.176 | ng/u1 | 0.00     |
| 15) 4-Methylphenol-d8         | 8.716  | 113  | 478439   | 13.535 | ng/u1 | 0.00     |
| 21) Nitrobenzene-d5           | 9.181  | 128  | 490269   | 33.131 | ng/u1 | 0.00     |
| 24) 2-Nitrophenol-d4          | 9.911  | 143  | 499360   | 31.781 | ng/u1 | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 10.446 | 165  | 930476   | 25.380 | ng/u1 | 0.00     |
| 31) 4-Chloroaniline-d4        | 10.963 | 131  | 1282506  | 25.546 | ng/u1 | 0.00     |
| 46) Dimethylphthalate-d6      | 14.057 | 166  | 3780334  | 33.270 | ng/u1 | 0.00     |
| 49) Acenaphthylene-d8         | 14.346 | 160  | 4203990  | 31.709 | ng/u1 | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.828 | 143  | 78186    | 3.860  | ng/u1 | 0.00     |
| 60) Fluorene-d10              | 15.646 | 176  | 3398433  | 34.152 | ng/u1 | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.751 | 200  | 430919   | 24.567 | ng/u1 | 0.00     |
| 73) Anthracene-d10            | 17.510 | 188  | 5610183  | 34.727 | ng/u1 | 0.00     |
| 81) Pyrene-d10                | 19.734 | 212  | 6636944  | 31.441 | ng/u1 | 0.00     |
| 92) Benzo(a)pyrene-d12        | 23.845 | 264  | 6210922  | 34.879 | ng/u1 | 0.00     |
| Target Compounds              |        |      |          |        |       |          |
| 2) 1,4-Dioxane                | 3.434  | 88   | 82737    | 6.183  | ng/uL | 93       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP112522\  
Data File : BP012785.D  
Acq On : 27 Nov 2022 01:32  
Operator : CG/JU  
Sample : N5710-04  
Misc :  
ALS Vial : 59 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
C0KY3

Quant Time: Nov 27 23:02:11 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP112522.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sun Nov 27 22:55:08 2022  
Response via : Initial Calibration

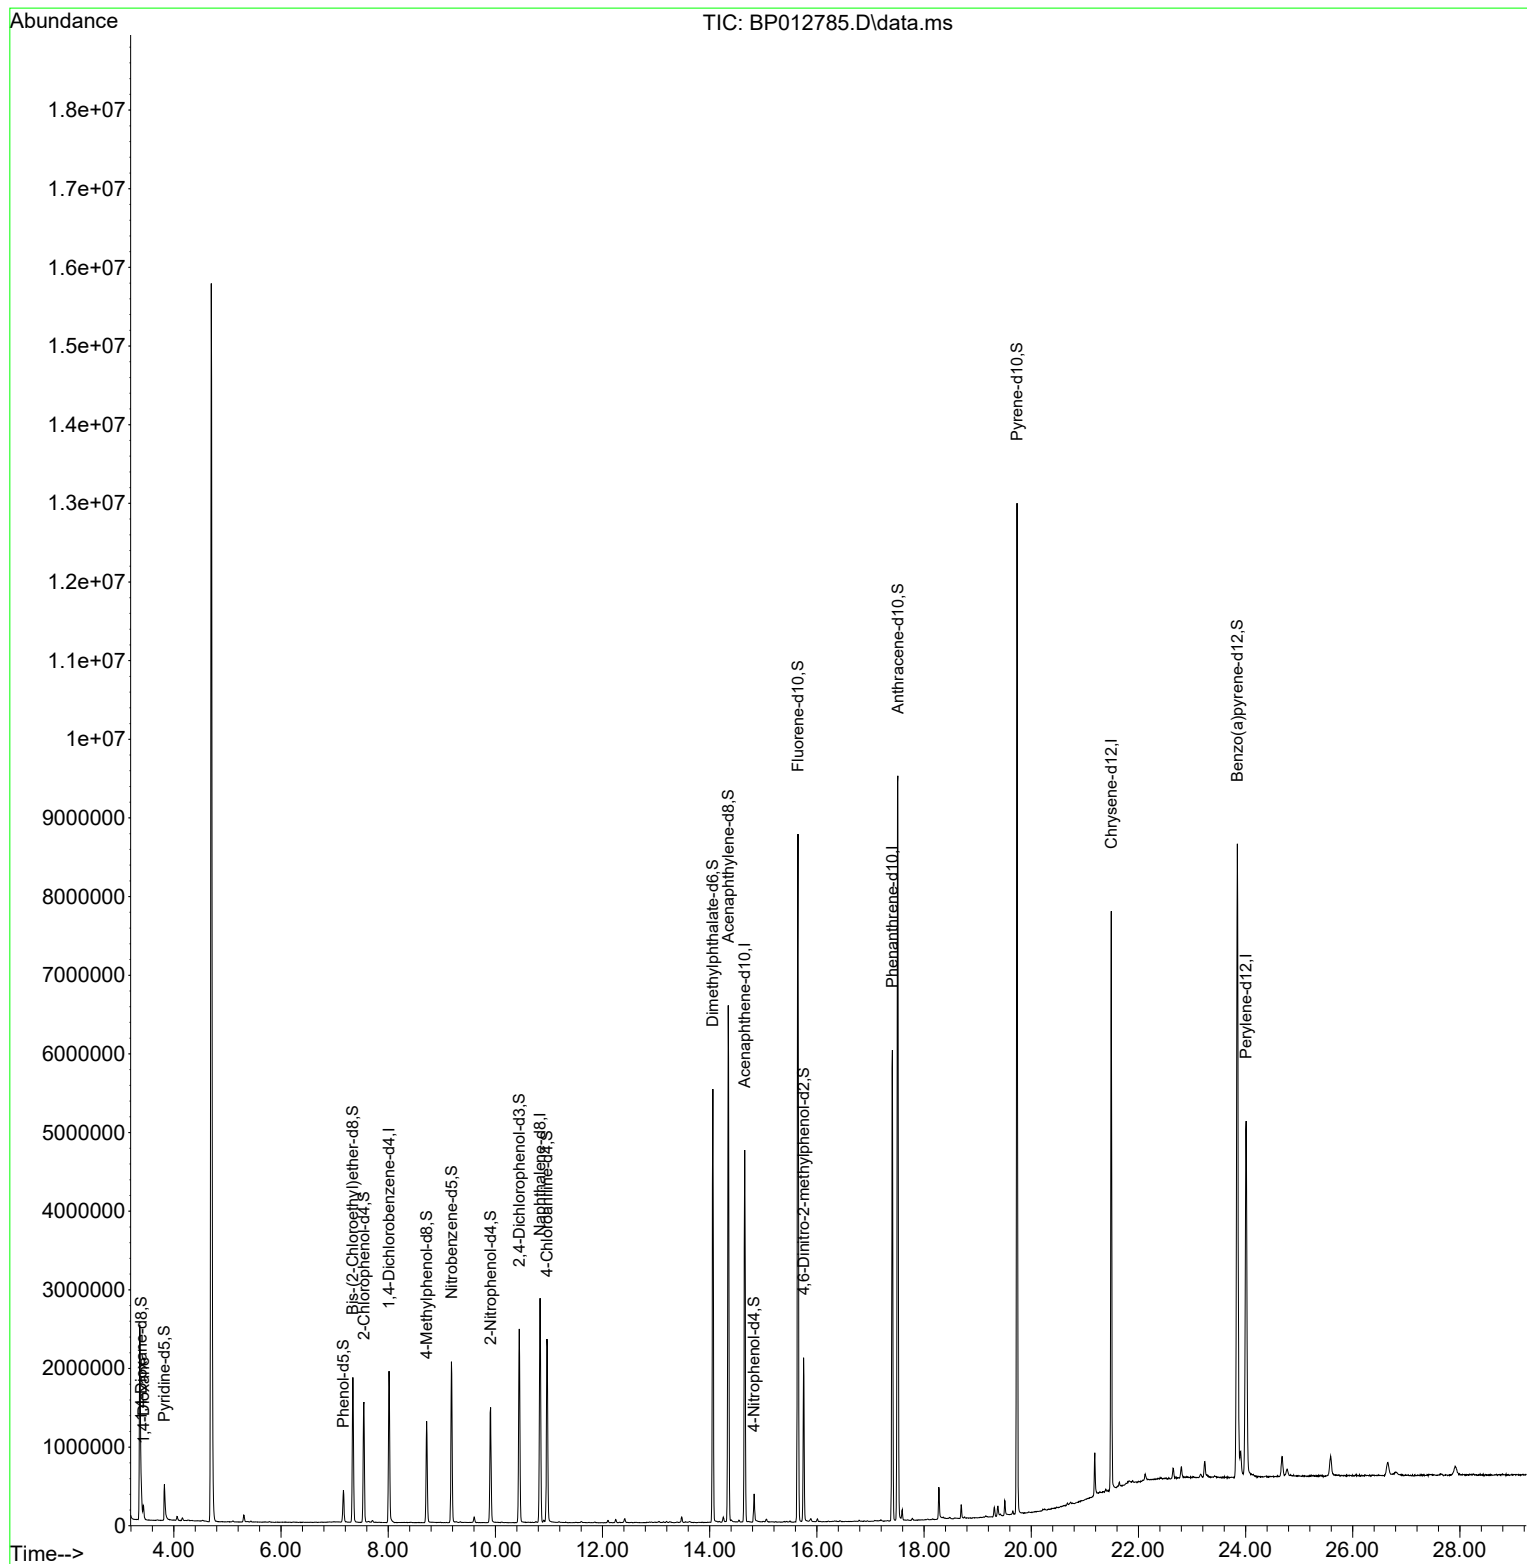

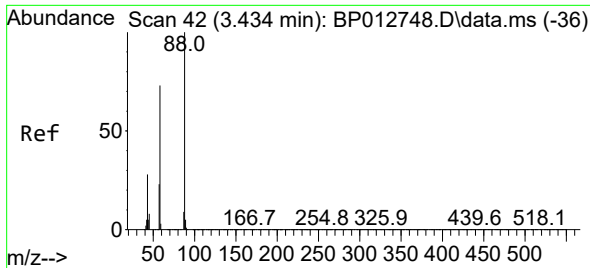

#2  
 1,4-Dioxane  
 Concen: 6.183 ng/uL  
 RT: 3.434 min Scan# 41  
 Delta R.T. 0.000 min  
 Lab File: BP012785.D  
 Acq: 27 Nov 2022 01:32

Instrument :  
 BNA\_P  
 ClientSampleId :  
 C0KY3

Tgt Ion: 88 Resp: 82737  
 Ion Ratio Lower Upper  
 88 100  
 43 26.8 22.6 34.0  
 58 67.7 59.6 89.4

