

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012786.D
 Acq On : 27 Nov 2022 02:07
 Operator : CG/JU
 Sample : N5710-05
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KY4

Quant Time: Nov 27 23:02:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	475836	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	2172353	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.651	164	1486303	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.404	188	3296588	20.000	ng/ul	0.00
79) Chrysene-d12	21.492	240	3233275	20.000	ng/ul	0.00
88) Perylene-d12	24.010	264	3214258	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	44560	4.013	ng/uL	0.00
4) Pyridine-d5	3.823	84	271598	8.173	ng/ul	0.00
7) Phenol-d5	7.164	99	249750	6.387	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	808835	33.570	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	765758	25.702	ng/ul	0.00
15) 4-Methylphenol-d8	8.716	113	523446	16.615	ng/ul	0.00
21) Nitrobenzene-d5	9.181	128	496005	37.305	ng/ul	0.00
24) 2-Nitrophenol-d4	9.910	143	481378	34.097	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.446	165	1010859	30.687	ng/ul	0.00
31) 4-Chloroaniline-d4	10.963	131	1267582	28.101	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	4034342	39.434	ng/ul	0.00
49) Acenaphthylene-d8	14.346	160	4220989	35.361	ng/ul	0.00
54) 4-Nitrophenol-d4	14.834	143	76019	4.168	ng/ul	0.00
60) Fluorene-d10	15.645	176	3459567	38.613	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	277468	17.610	ng/ul	0.00
73) Anthracene-d10	17.504	188	5821019	40.114	ng/ul	0.00
81) Pyrene-d10	19.733	212	6861806	36.524	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.845	264	6413016	40.619	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.193	94	98327	2.398	ng/ul	98
16) Acetophenone	8.840	105	84717	1.697	ng/ul	99
59) Diethylphthalate	15.469	149	1711660	16.489	ng/ul	99
78) Di-n-butylphthalate	18.351	149	411787	2.366	ng/ul#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012786.D
Acq On : 27 Nov 2022 02:07
Operator : CG/JU
Sample : N5710-05
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COKY4

Quant Time: Nov 27 23:02:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration




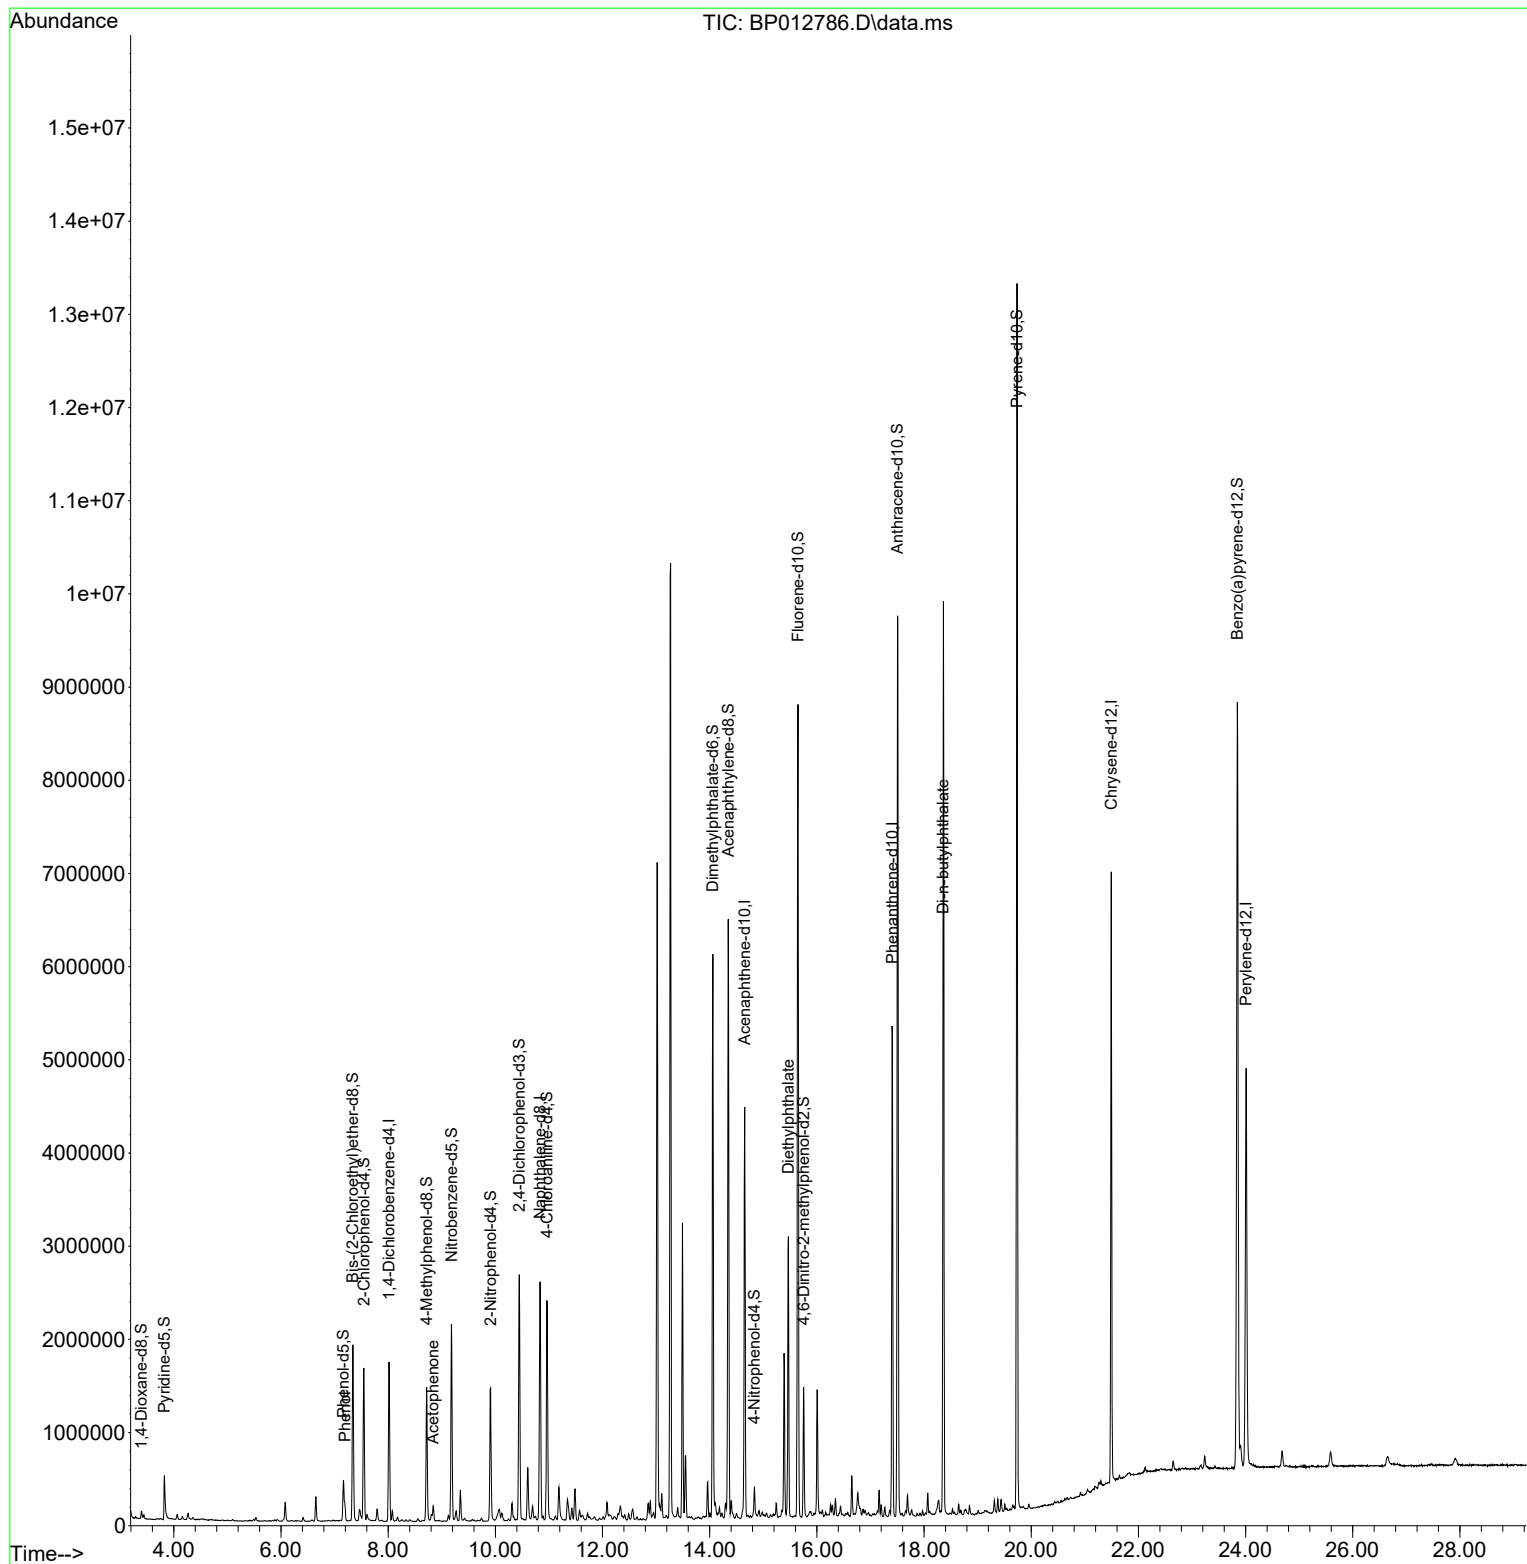


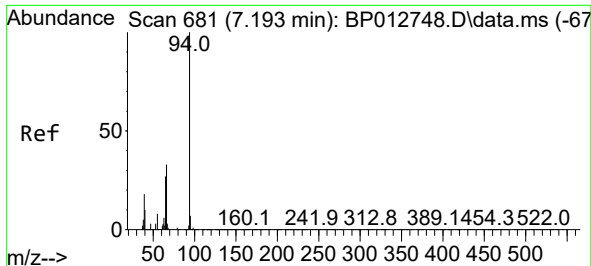

#8
Phenol
Concen: 2.398 ng/ul
RT: 7.193 min Scan# 681
Delta R.T. 0.000 min
Lab File: BP012786.D
Acq: 27 Nov 2022 02:07




Instrument :
BNA_P
ClientSampleId :
C0KY4


Tgt Ion: 94 Resp: 98327
Ion Ratio Lower Upper
94 100
65 25.7 20.9 31.3
66 33.7 26.0 39.0

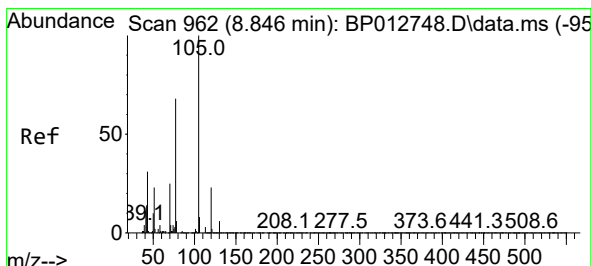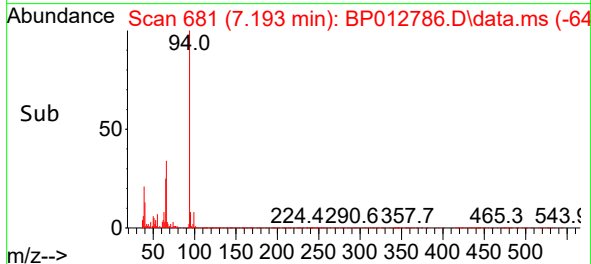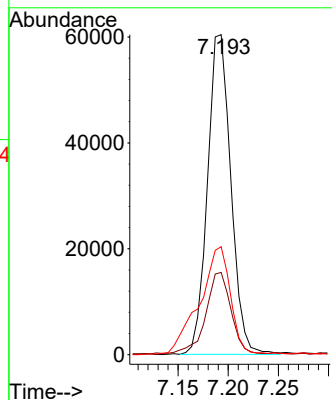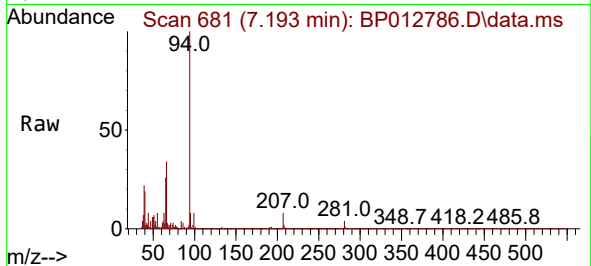

#16
Acetophenone
Concen: 1.697 ng/ul
RT: 8.840 min Scan# 961
Delta R.T. -0.006 min
Lab File: BP012786.D
Acq: 27 Nov 2022 02:07

Tgt Ion: 105 Resp: 84717
Ion Ratio Lower Upper
105 100
77 75.1 59.7 89.5
51 26.7 20.9 31.3


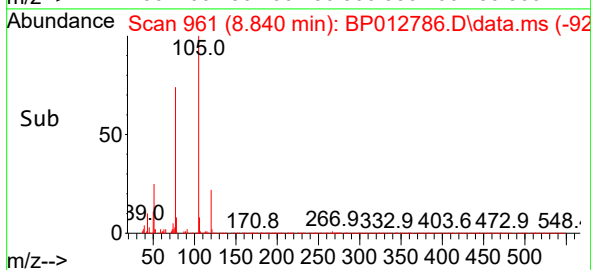
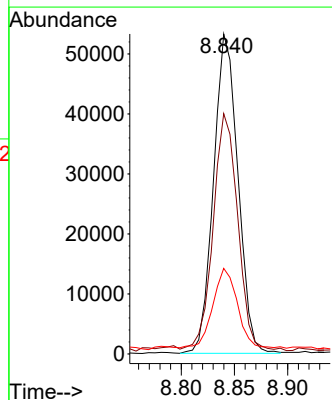
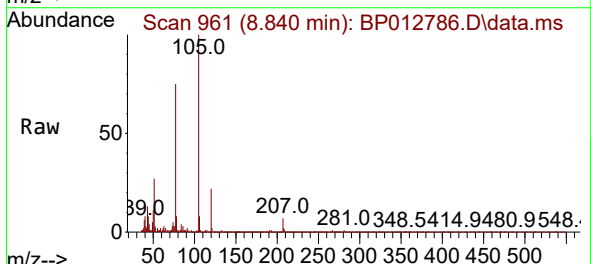


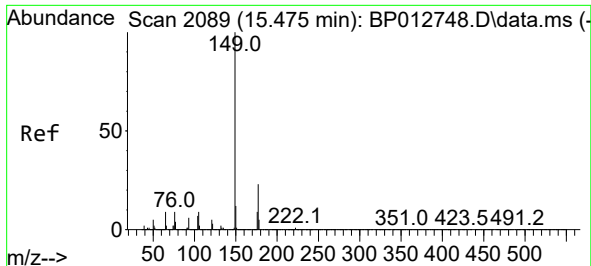

#59
Diethylphthalate
Concen: 16.489 ng/ul
RT: 15.469 min Scan# 2088
Delta R.T. -0.006 min
Lab File: BP012786.D
Acq: 27 Nov 2022 02:07

Instrument :
BNA_P
ClientSampleId :
C0KY4

Tgt Ion:149 Resp: 1711660
Ion Ratio Lower Upper
149 100
177 22.9 18.1 27.1
150 12.1 9.8 14.8

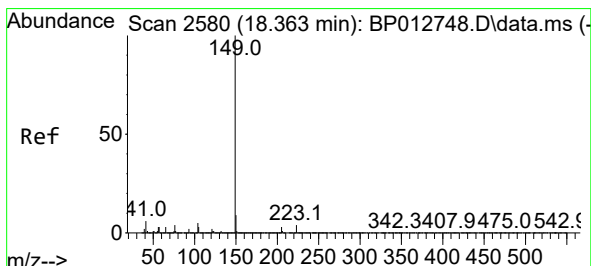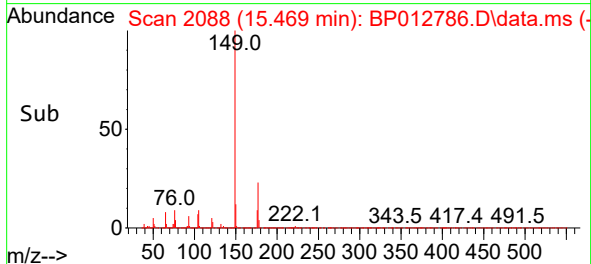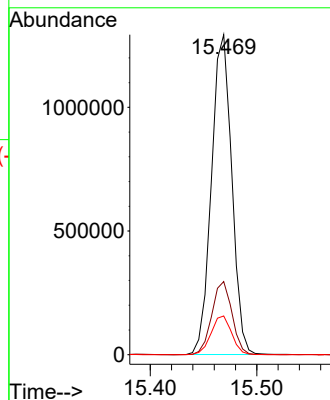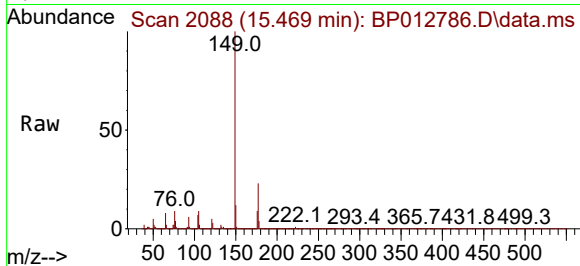

#78
Di-n-butylphthalate
Concen: 2.366 ng/ul
RT: 18.351 min Scan# 2578
Delta R.T. -0.006 min
Lab File: BP012786.D
Acq: 27 Nov 2022 02:07

Tgt Ion:149 Resp: 411787
Ion Ratio Lower Upper
149 100
150 11.8 7.2 10.8#
104 5.0 3.7 5.5

