

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012790.D
 Acq On : 27 Nov 2022 04:23
 Operator : CG/JU
 Sample : N5710-10
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KY9

Quant Time: Nov 27 23:03:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	568031	20.000	ng/u1	0.00
20) Naphthalene-d8	10.834	136	2535051	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.651	164	1707805	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.410	188	3810958	20.000	ng/u1	0.00
79) Chrysene-d12	21.492	240	3893128	20.000	ng/u1	0.00
88) Perylene-d12	24.009	264	3850036	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	64717	4.882	ng/uL	0.00
4) Pyridine-d5	3.822	84	275325	6.940	ng/u1	0.00
7) Phenol-d5	7.163	99	326181	6.988	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	766301	26.643	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	763056	21.454	ng/u1	0.00
15) 4-Methylphenol-d8	8.716	113	545959	14.517	ng/u1	0.00
21) Nitrobenzene-d5	9.181	128	466314	30.054	ng/u1	0.00
24) 2-Nitrophenol-d4	9.910	143	466414	28.310	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.445	165	943491	24.544	ng/u1	0.00
31) 4-Chloroaniline-d4	10.963	131	966512	18.361	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	3664025	31.170	ng/u1	0.00
49) Acenaphthylene-d8	14.345	160	4052734	29.548	ng/u1	0.00
54) 4-Nitrophenol-d4	14.833	143	141125	6.734	ng/u1	0.00
60) Fluorene-d10	15.645	176	3246492	31.535	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	449298	24.667	ng/u1	0.00
73) Anthracene-d10	17.510	188	5444217	32.453	ng/u1	0.00
81) Pyrene-d10	19.733	212	6551047	28.960	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.845	264	6175074	32.653	ng/u1	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.434	88	1116999	78.462	ng/uL	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012790.D
Acq On : 27 Nov 2022 04:23
Operator : CG/JU
Sample : N5710-10
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KY9

Quant Time: Nov 27 23:03:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration

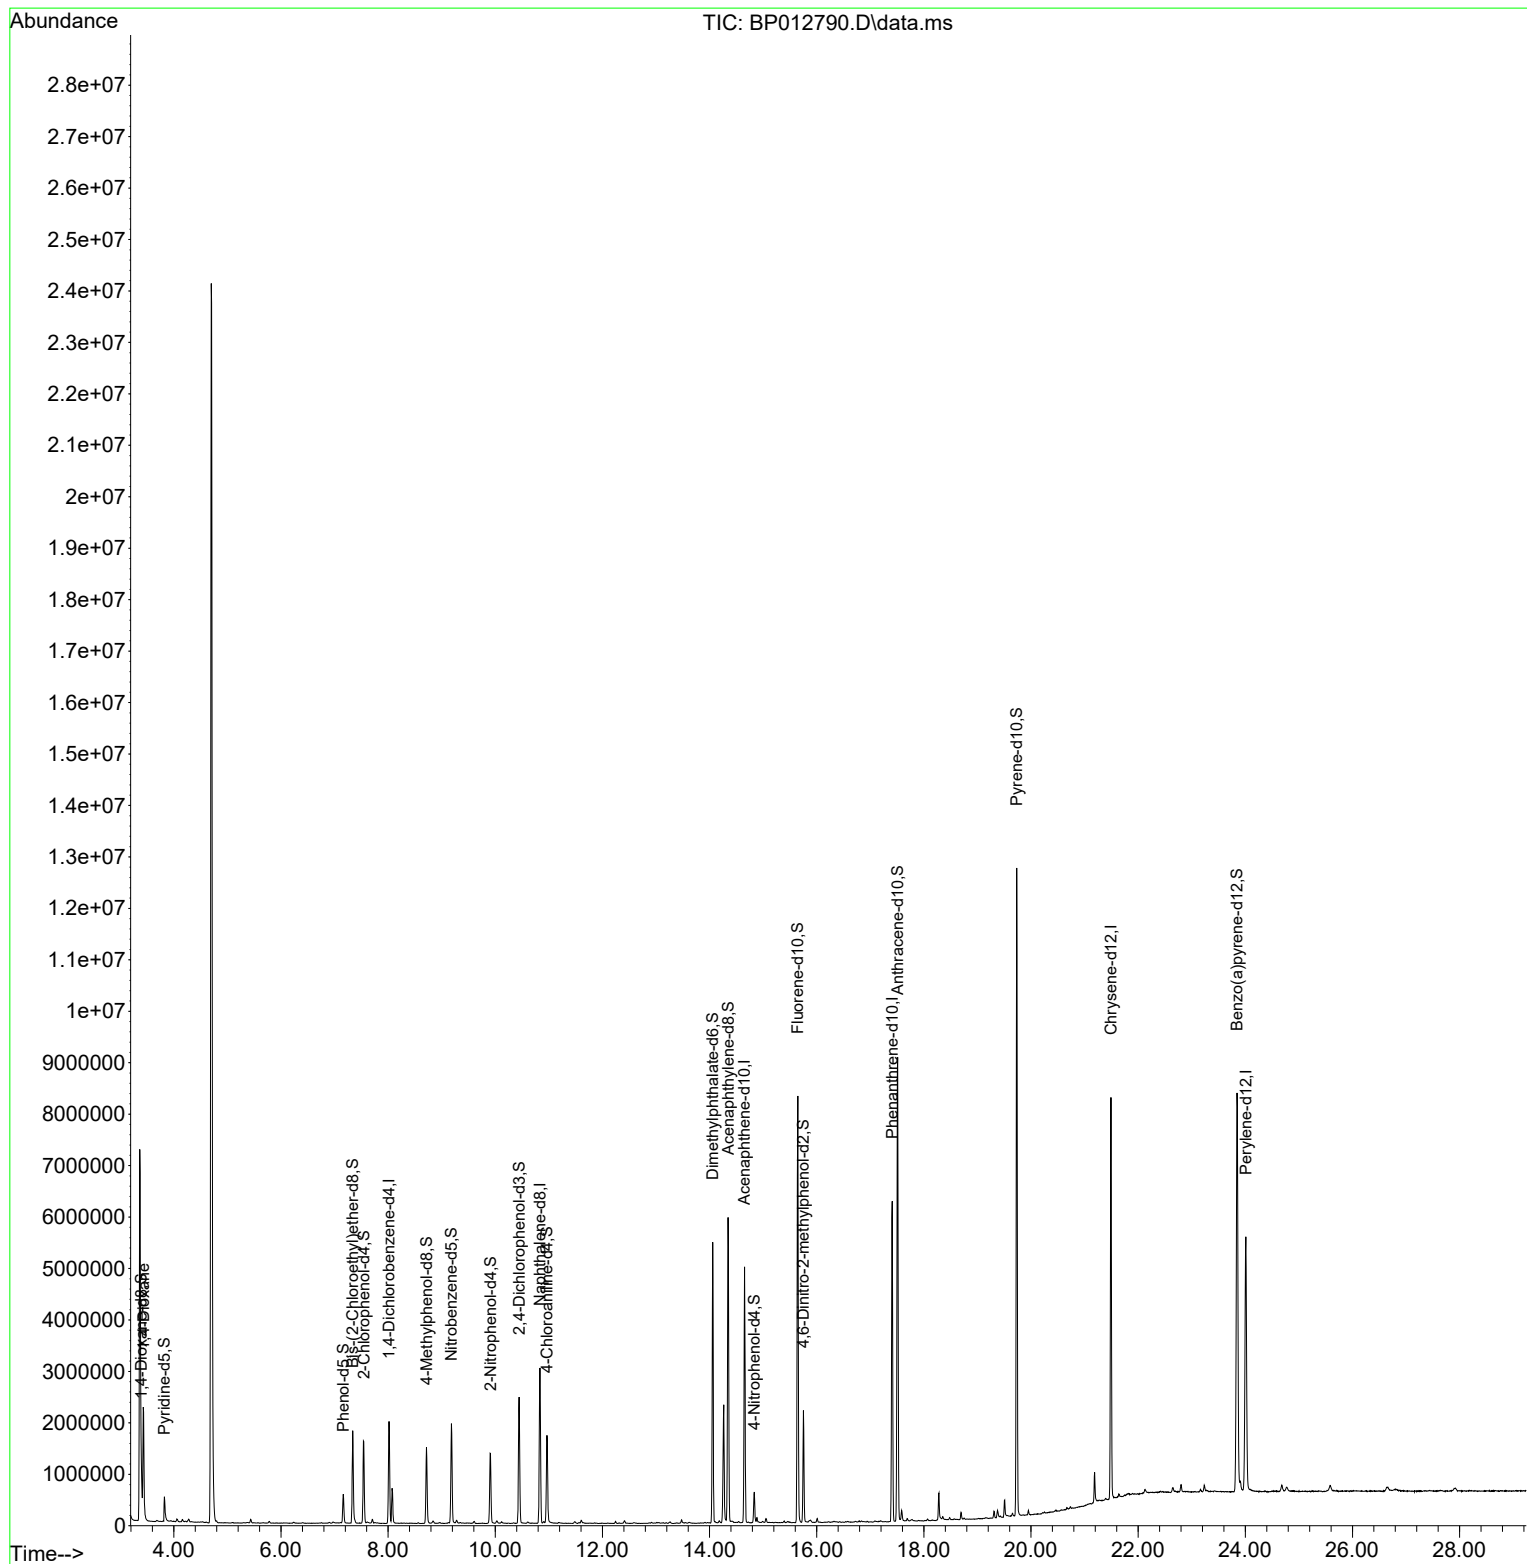

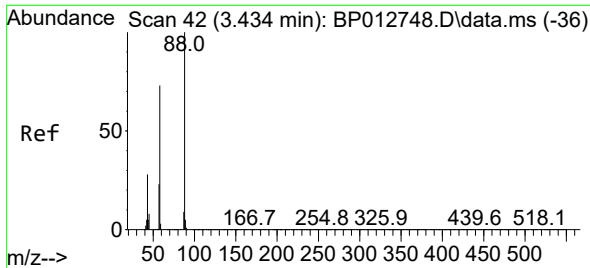

#2
 1,4-Dioxane
 Concen: 78.462 ng/uL
 RT: 3.434 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BP012790.D
 Acq: 27 Nov 2022 04:23

Instrument :
 BNA_P
 ClientSampleId :
 C0KY9

Tgt Ion: 88 Resp: 1116999
 Ion Ratio Lower Upper
 88 100
 43 25.6 22.6 34.0
 58 70.2 59.6 89.4

