

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012792.D
 Acq On : 27 Nov 2022 05:31
 Operator : CG/JU
 Sample : N5710-17
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0L03

Quant Time: Nov 27 23:03:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	558033	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	2543657	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.651	164	1741103	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.410	188	3858213	20.000	ng/ul	0.00
79) Chrysene-d12	21.492	240	3829240	20.000	ng/ul	0.00
88) Perylene-d12	24.010	264	3849415	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	55252	4.243	ng/uL	0.00
4) Pyridine-d5	3.822	84	275270	7.063	ng/ul	0.00
7) Phenol-d5	7.163	99	298756	6.515	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	862936	30.540	ng/ul	0.00
11) 2-Chlorophenol-d4	7.540	132	847099	24.244	ng/ul	0.00
15) 4-Methylphenol-d8	8.716	113	590249	15.976	ng/ul	0.00
21) Nitrobenzene-d5	9.181	128	541466	34.779	ng/ul	0.00
24) 2-Nitrophenol-d4	9.910	143	535637	32.402	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.446	165	1083487	28.090	ng/ul	0.00
31) 4-Chloroaniline-d4	10.963	131	1372281	25.981	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	4086252	34.097	ng/ul	0.00
49) Acenaphthylene-d8	14.345	160	4492120	32.125	ng/ul	0.00
54) 4-Nitrophenol-d4	14.834	143	98022	4.588	ng/ul	0.00
60) Fluorene-d10	15.645	176	3576271	34.074	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	388354	21.060	ng/ul	0.00
73) Anthracene-d10	17.504	188	5960278	35.095	ng/ul	0.00
81) Pyrene-d10	19.733	212	7087978	31.856	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.845	264	6751344	35.706	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.193	94	107145	2.228	ng/ul	95
16) Acetophenone	8.840	105	88522	1.512	ng/ul	99
59) Diethylphthalate	15.469	149	1749579	14.388	ng/ul	99
78) Di-n-butylphthalate	18.351	149	440820	2.164	ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012792.D
Acq On : 27 Nov 2022 05:31
Operator : CG/JU
Sample : N5710-17
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COL03

Quant Time: Nov 27 23:03:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration




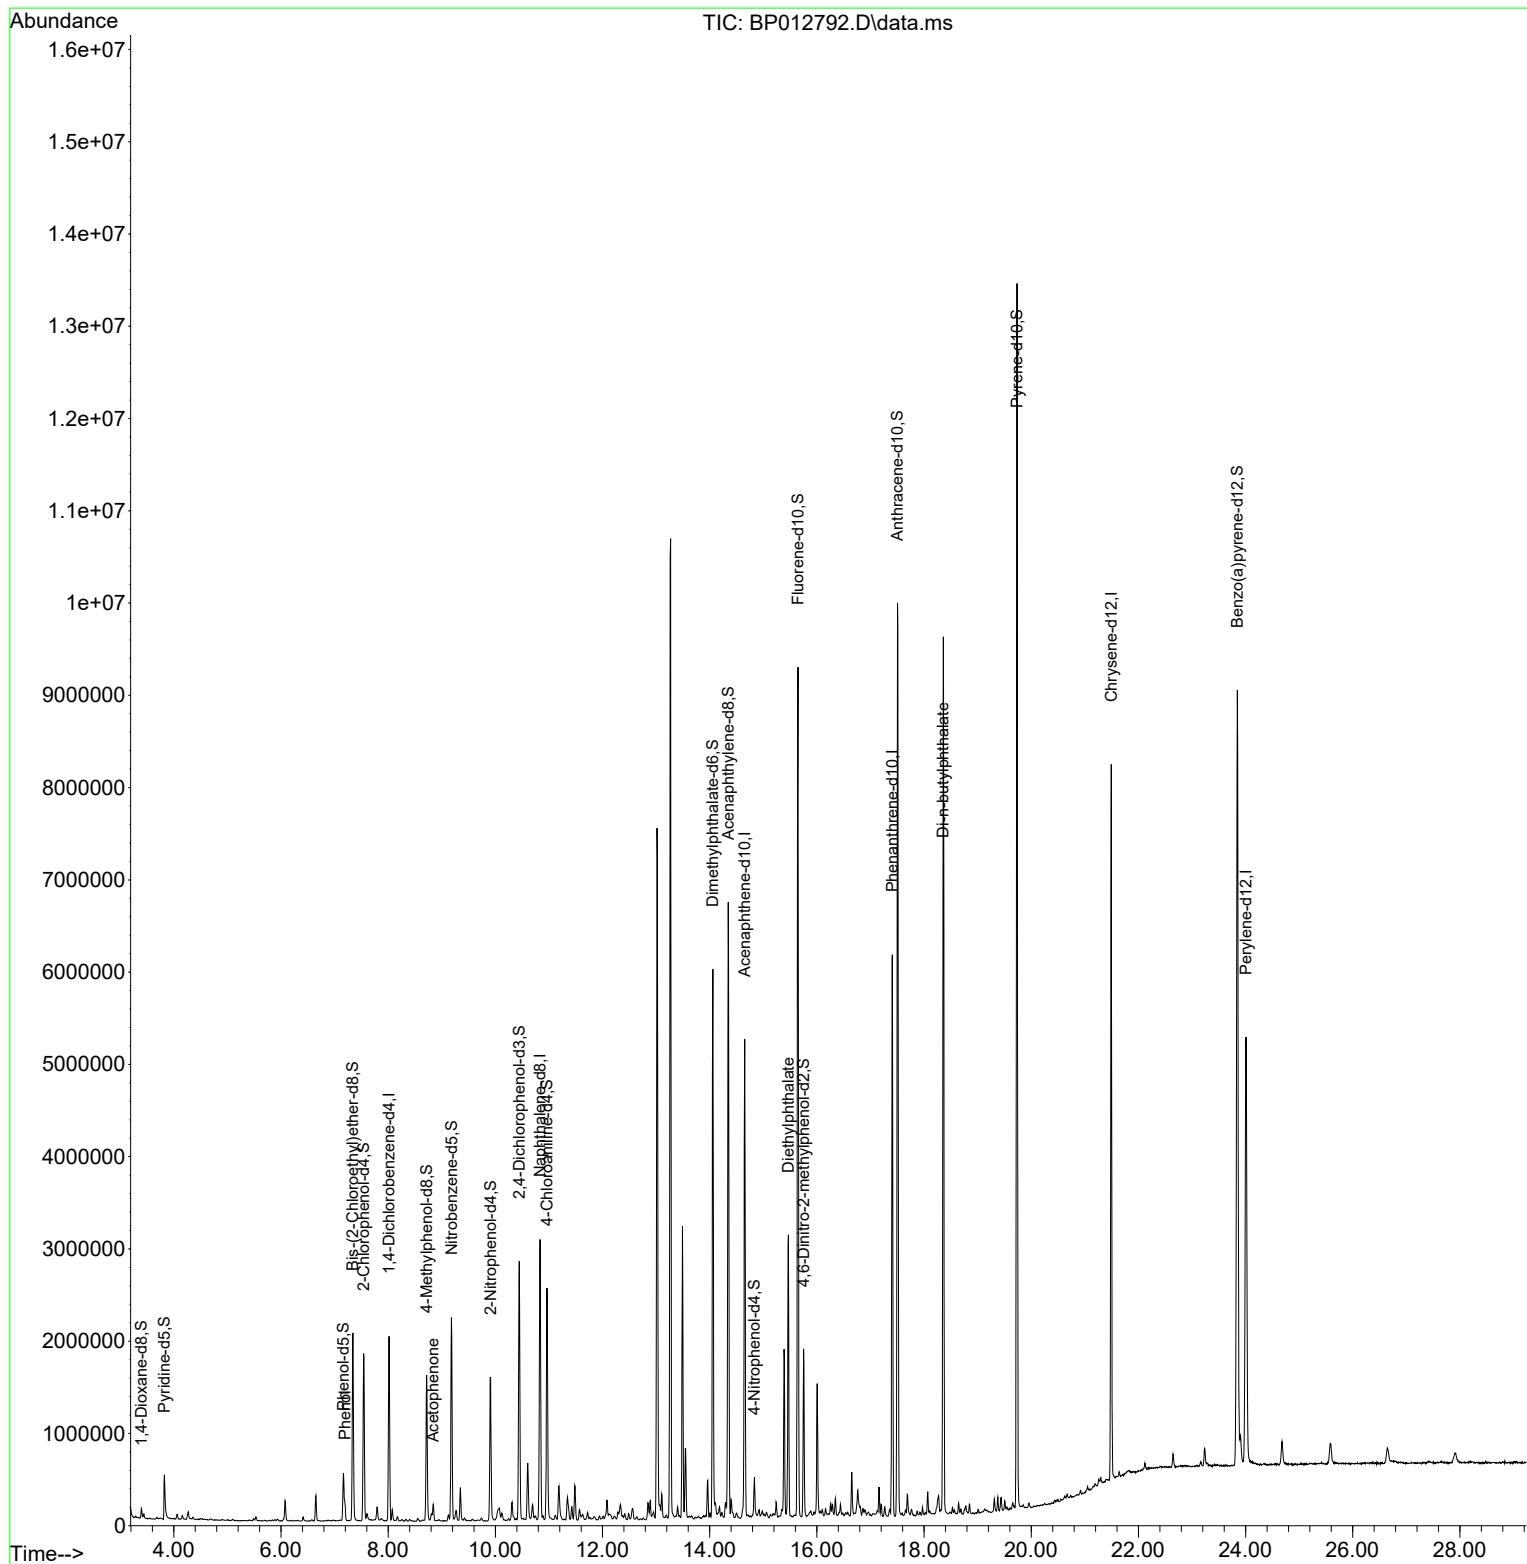


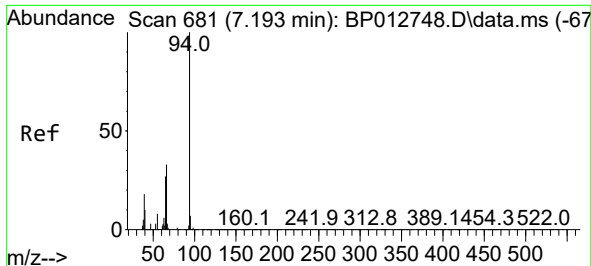

#8
Phenol
Concen: 2.228 ng/ul
RT: 7.193 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP012792.D
Acq: 27 Nov 2022 05:31




Instrument :
BNA_P
ClientSampleId :
COL03


Tgt Ion: 94 Resp: 107145
Ion Ratio Lower Upper
94 100
65 27.9 20.9 31.3
66 35.8 26.0 39.0

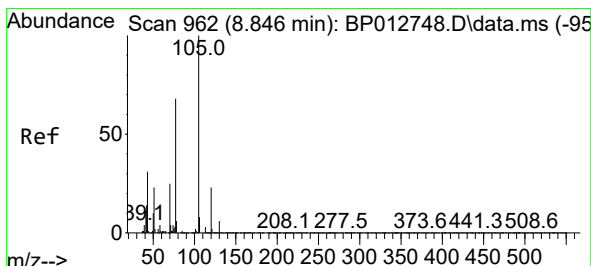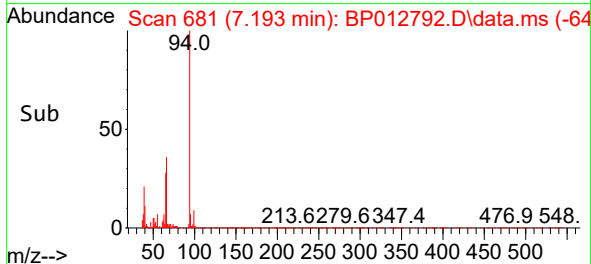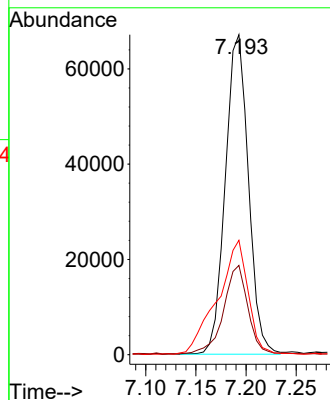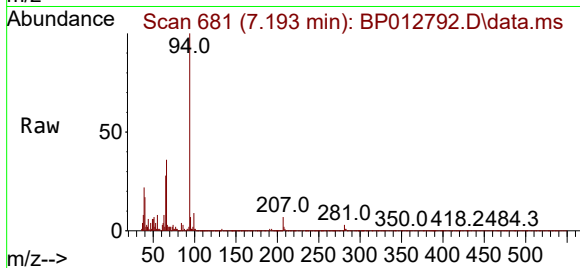

#16
Acetophenone
Concen: 1.512 ng/ul
RT: 8.840 min Scan# 961
Delta R.T. -0.006 min
Lab File: BP012792.D
Acq: 27 Nov 2022 05:31

Tgt Ion: 105 Resp: 88522
Ion Ratio Lower Upper
105 100
77 74.9 59.7 89.5
51 28.3 20.9 31.3


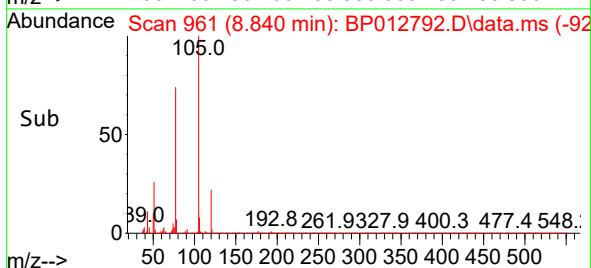
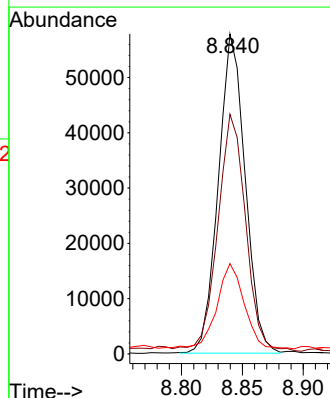
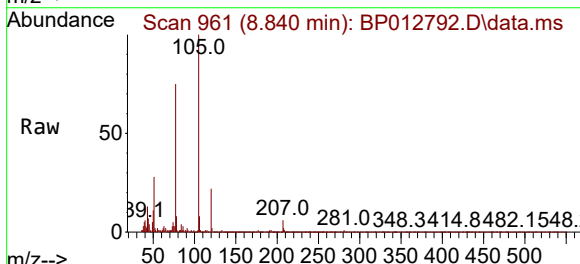


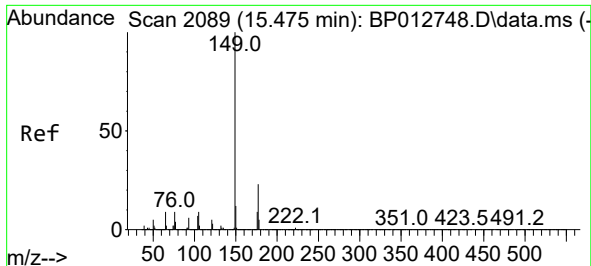

#59
Diethylphthalate
Concen: 14.388 ng/ul
RT: 15.469 min Scan# 2088
Delta R.T. -0.006 min
Lab File: BP012792.D
Acq: 27 Nov 2022 05:31

Instrument :
BNA_P
ClientSampleId :
COL03

Tgt Ion:149 Resp: 1749579
Ion Ratio Lower Upper
149 100
177 23.5 18.1 27.1
150 12.3 9.8 14.8

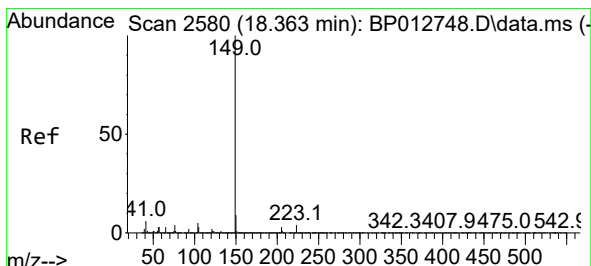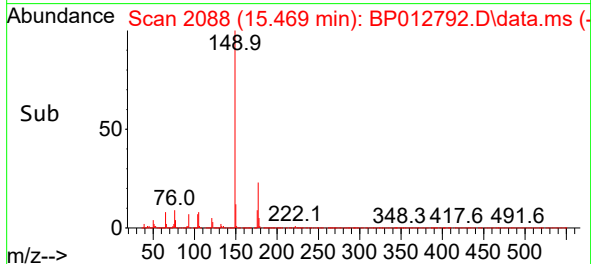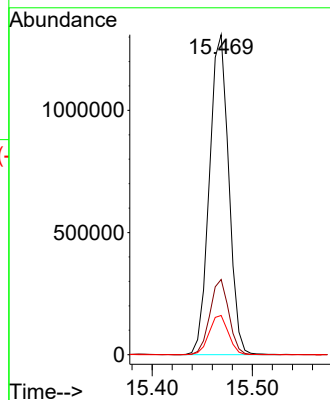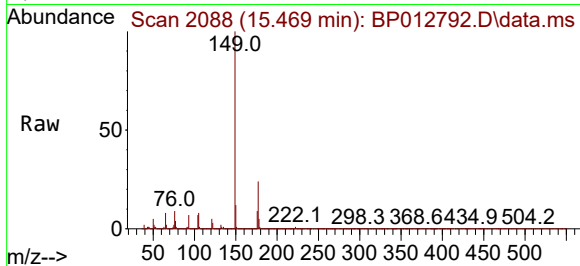

#78
Di-n-butylphthalate
Concen: 2.164 ng/ul
RT: 18.351 min Scan# 2578
Delta R.T. -0.006 min
Lab File: BP012792.D
Acq: 27 Nov 2022 05:31

Tgt Ion:149 Resp: 440820
Ion Ratio Lower Upper
149 100
150 11.8 7.2 10.8#
104 4.6 3.7 5.5

