




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012789.D
Acq On : 27 Nov 2022 03:49
Operator : CG/JU
Sample : N5710-09
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KY8

Manual IntegrationsAPPROVED

Quant Time: Nov 27 23:02:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/28/2022
Supervised By :mohammad ahmed 11/30/2022

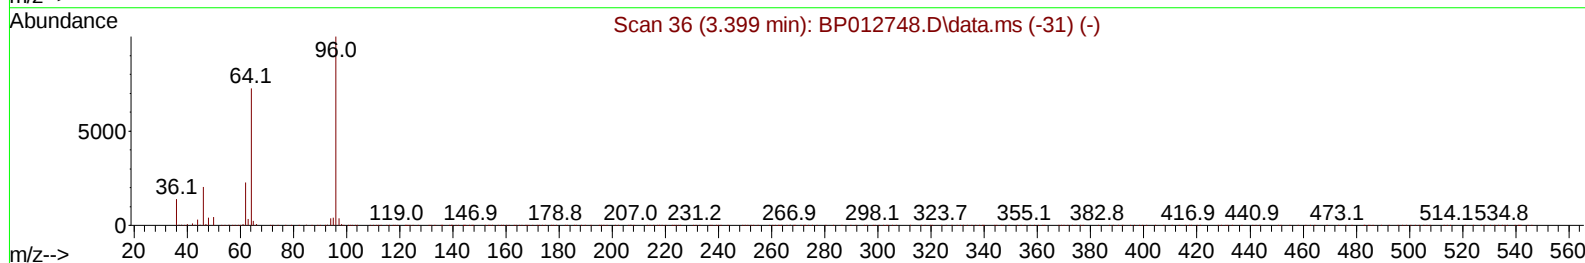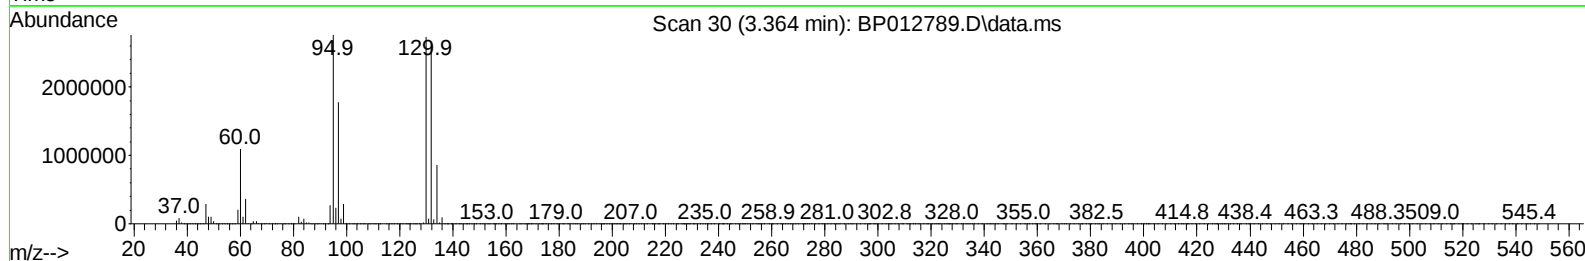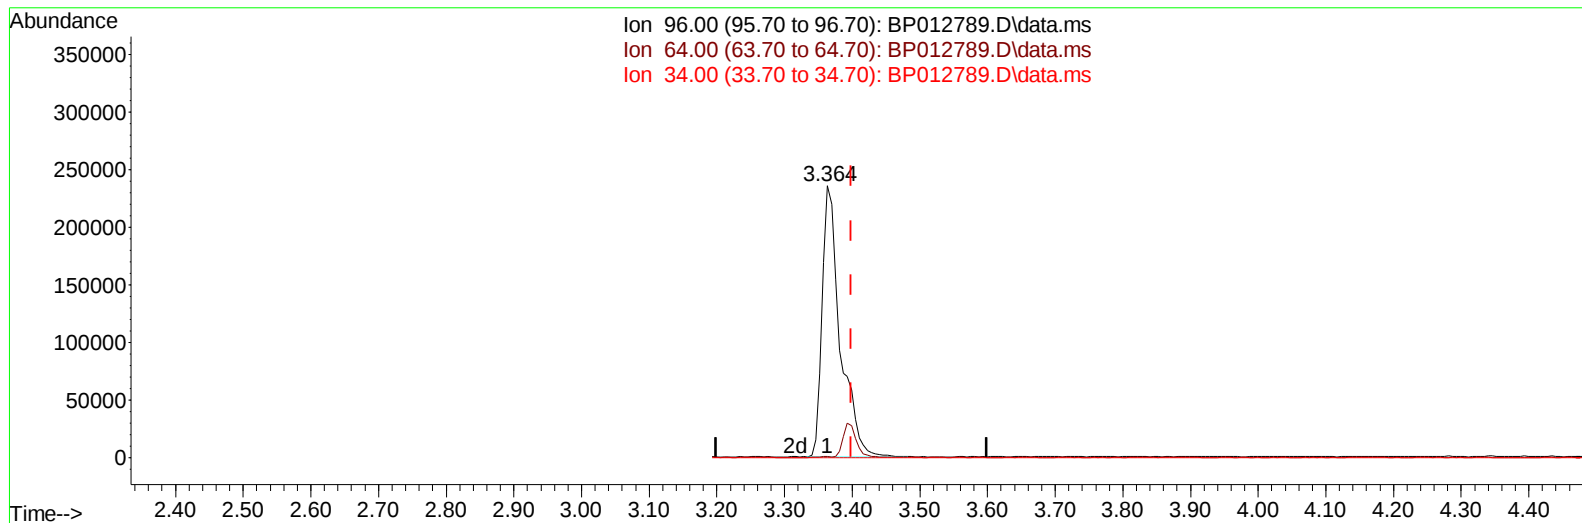

TIC: BP012789.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.364min (-0.035) 34.14 ng/uL

response 438993

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.90	0.35#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012789.D
 Acq On : 27 Nov 2022 03:49
 Operator : CG/JU
 Sample : N5710-09
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KY8

Manual IntegrationsAPPROVED

Quant Time: Nov 27 23:02:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/28/2022
 Supervised By :mohammad ahmed 11/30/2022

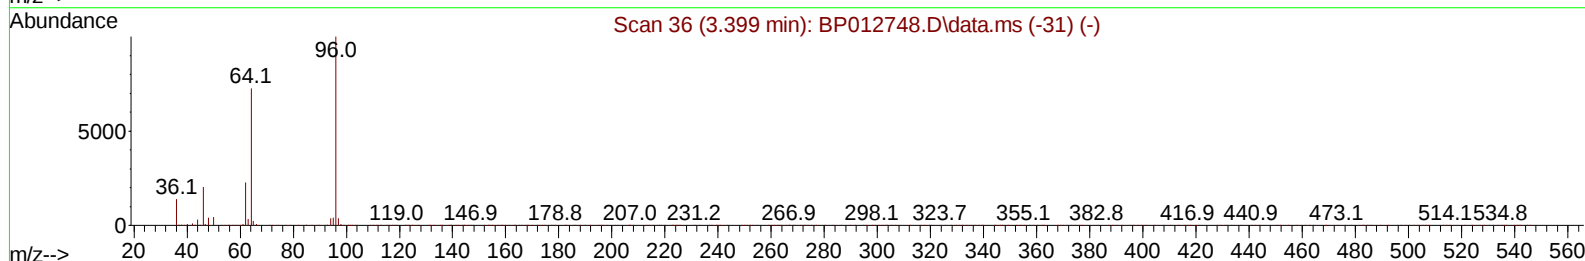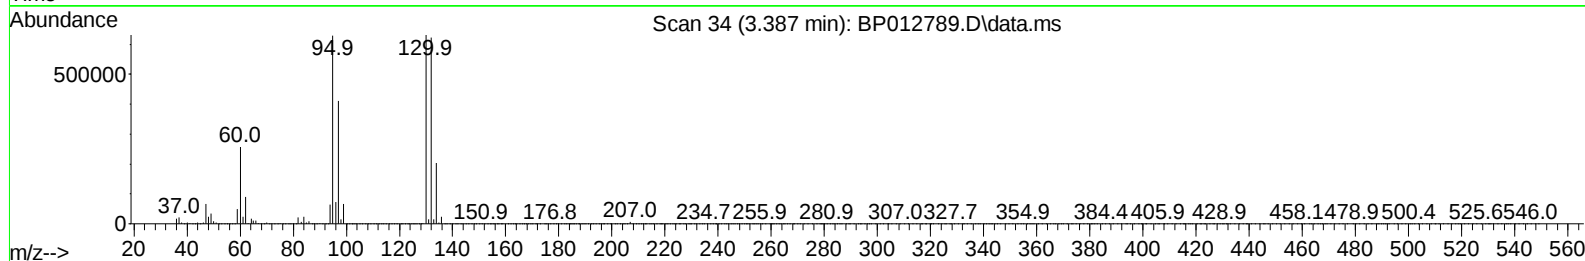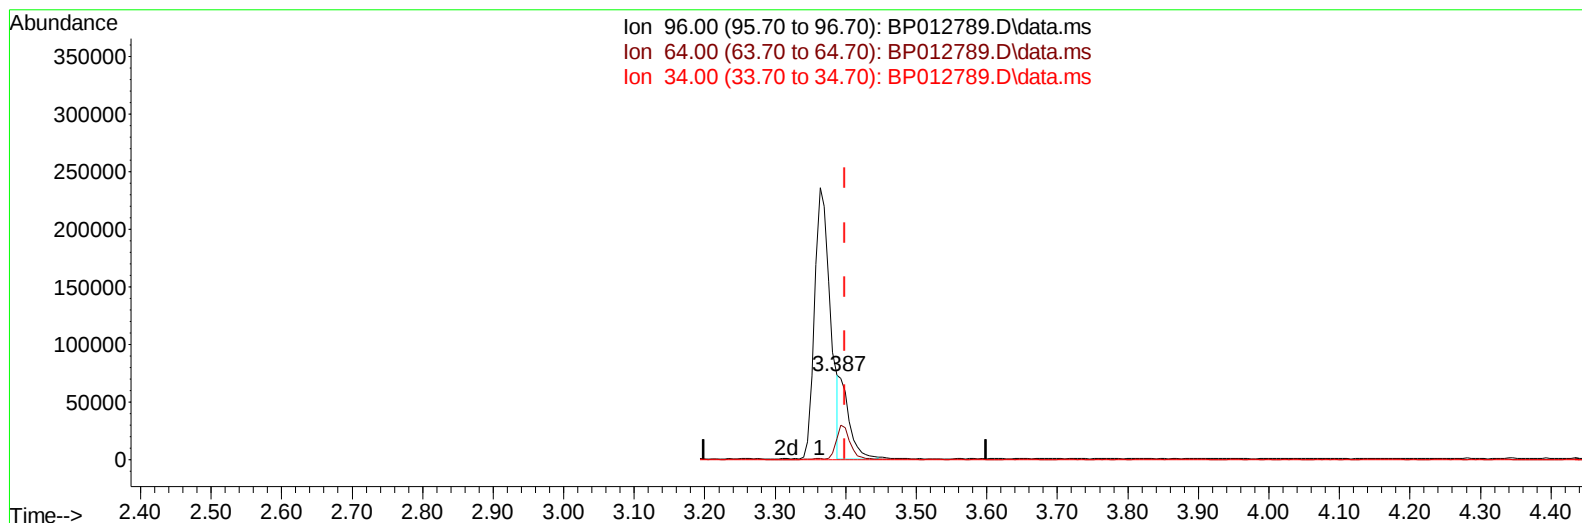

TIC: BP012789.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.387min (-0.012) 5.63 ng/uL m

response 72356

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.90	24.59#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012789.D
 Acq On : 27 Nov 2022 03:49
 Operator : CG/JU
 Sample : N5710-09
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KY8

Manual IntegrationsAPPROVED

Quant Time: Nov 27 23:02:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/28/2022
 Supervised By :mohammad ahmed 11/30/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	551081	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	2464696	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.651	164	1670536	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.404	188	3698404	20.000	ng/ul	0.00
79) Chrysene-d12	21.492	240	3664068	20.000	ng/ul	0.00
88) Perylene-d12	24.010	264	3660028	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	72356m	5.626	ng/uL	-0.01
4) Pyridine-d5	3.834	84	50085	1.301	ng/ul	0.01
7) Phenol-d5	7.163	99	275966	6.094	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	809058	28.995	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	793012	22.982	ng/ul	0.00
15) 4-Methylphenol-d8	8.716	113	504795	13.835	ng/ul	0.00
21) Nitrobenzene-d5	9.181	128	484343	32.107	ng/ul	0.00
24) 2-Nitrophenol-d4	9.910	143	502549	31.374	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.446	165	953877	25.522	ng/ul	0.00
31) 4-Chloroaniline-d4	10.963	131	426937	8.342	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	3606289	31.363	ng/ul	0.00
49) Acenaphthylene-d8	14.345	160	3312865	24.692	ng/ul	0.00
54) 4-Nitrophenol-d4	14.828	143	96682	4.716	ng/ul	0.00
60) Fluorene-d10	15.645	176	3201595	31.793	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	395116	22.353	ng/ul	0.00
73) Anthracene-d10	17.504	188	4974343	30.555	ng/ul	0.00
81) Pyrene-d10	19.733	212	6178659	29.021	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.845	264	5843774	32.506	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.428	88	958589	69.405	ng/uL	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012789.D
Acq On : 27 Nov 2022 03:49
Operator : CG/JU
Sample : N5710-09
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KY8

Manual IntegrationsAPPROVED

Quant Time: Nov 27 23:02:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/28/2022
Supervised By :mohammad ahmed 11/30/2022

