




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012806.D
Acq On : 27 Nov 2022 14:01
Operator : CG/JU
Sample : N5683-14
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ESQW7

Manual IntegrationsAPPROVED

Quant Time: Nov 27 23:08:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/28/2022
Supervised By :mohammad ahmed 11/30/2022

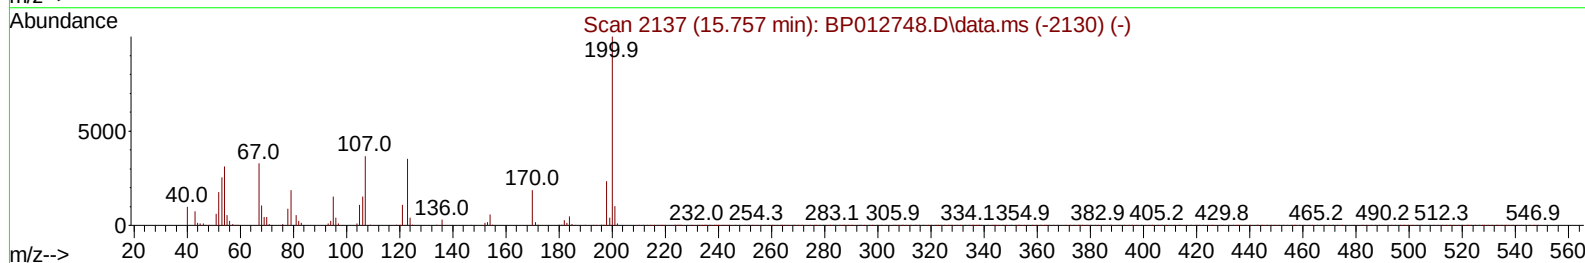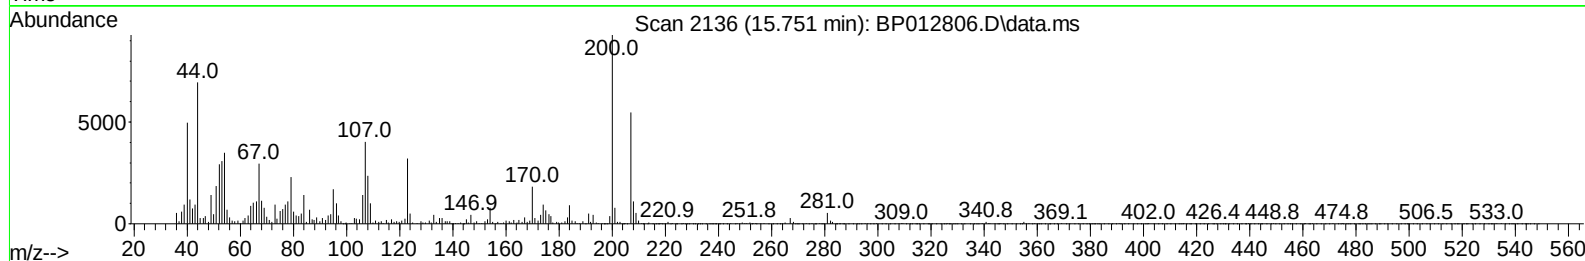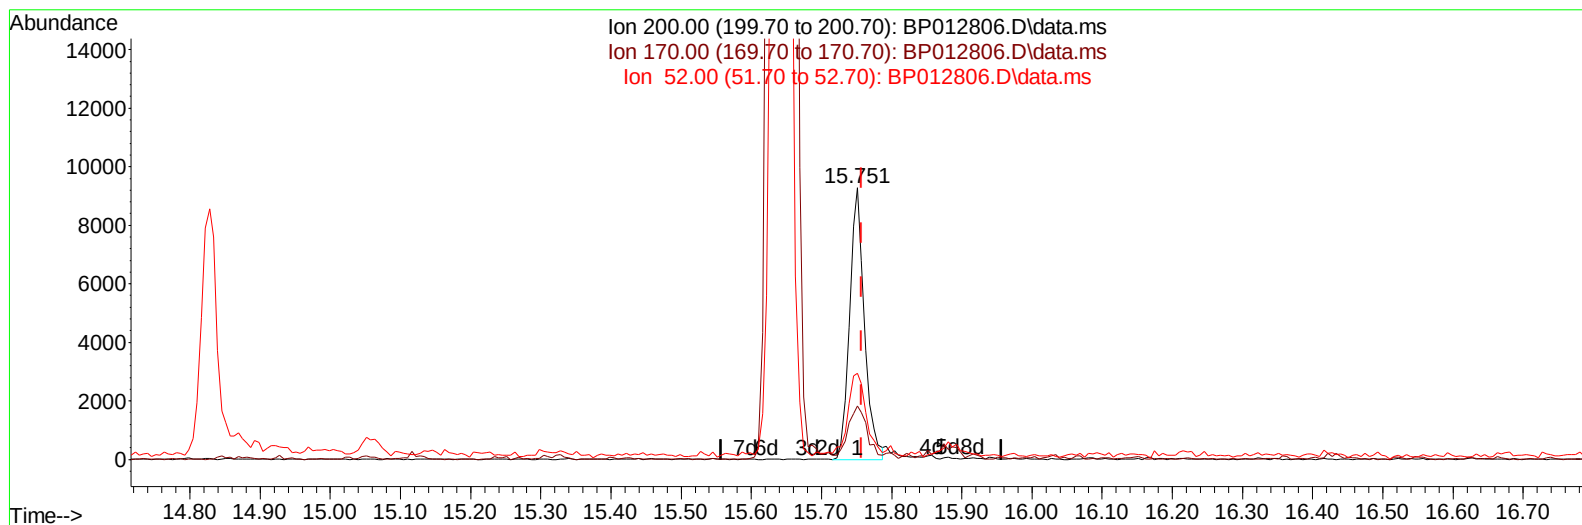

TIC: BP012806.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.751min (-0.006) 0.79 ng/ul

response 13673

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	17.20	19.63
52.00	38.80	31.68
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012806.D
 Acq On : 27 Nov 2022 14:01
 Operator : CG/JU
 Sample : N5683-14
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ESQW7

Manual IntegrationsAPPROVED

Quant Time: Nov 27 23:08:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/28/2022
 Supervised By :mohammad ahmed 11/30/2022

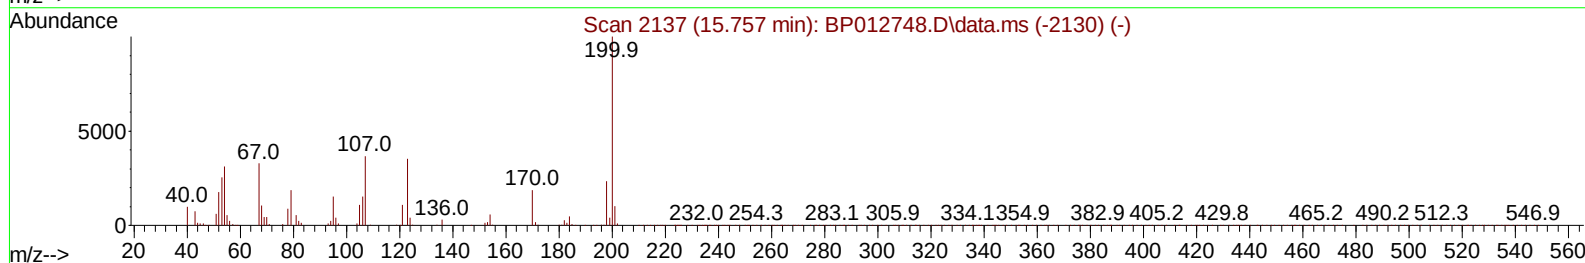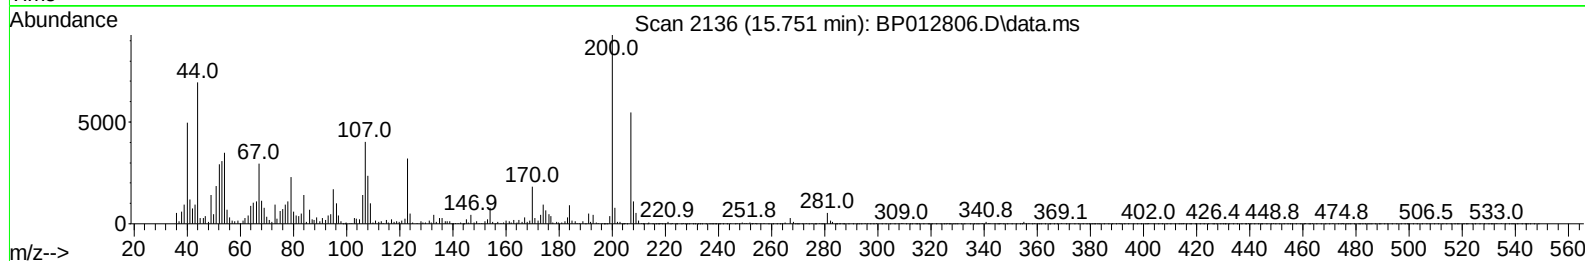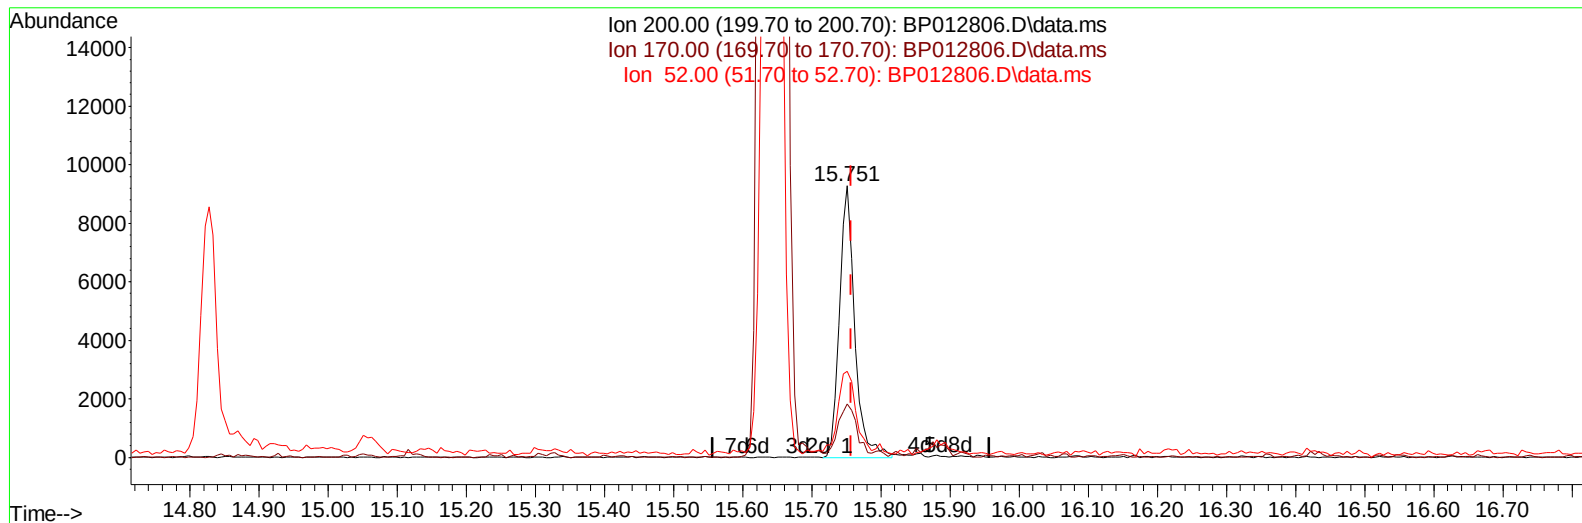

TIC: BP012806.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.751min (-0.006) 0.82 ng/ul m

response 14100

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	17.20	19.63
52.00	38.80	31.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012806.D
 Acq On : 27 Nov 2022 14:01
 Operator : CG/JU
 Sample : N5683-14
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ESQW7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/28/2022
 Supervised By :mohammad ahmed 11/30/2022

Quant Time: Nov 27 23:08:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	490924	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	2249597	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.651	164	1587574	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.404	188	3610865	20.000	ng/ul	0.00
79) Chrysene-d12	21.492	240	3770820	20.000	ng/ul	0.00
88) Perylene-d12	24.010	264	3881011	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	42353	3.697	ng/uL	0.00
4) Pyridine-d5	3.822	84	228732	6.672	ng/ul	0.00
7) Phenol-d5	7.163	99	551994	13.683	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	1033706	41.585	ng/ul	0.00
11) 2-Chlorophenol-d4	7.540	132	944144	30.715	ng/ul	0.00
15) 4-Methylphenol-d8	8.716	113	710322	21.854	ng/ul	0.00
21) Nitrobenzene-d5	9.181	128	686846	49.884	ng/ul	0.00
24) 2-Nitrophenol-d4	9.904	143	342511	23.428	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.446	165	1122773	32.914	ng/ul	0.00
31) 4-Chloroaniline-d4	10.963	131	1751926	37.504	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	5076768	46.458	ng/ul	0.00
49) Acenaphthylene-d8	14.345	160	5707078	44.761	ng/ul	0.00
54) 4-Nitrophenol-d4	14.828	143	113588	5.830	ng/ul	0.00
60) Fluorene-d10	15.645	176	4477442	46.786	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	14100m	0.817	ng/ul	0.00
73) Anthracene-d10	17.504	188	7291455	45.874	ng/ul	0.00
81) Pyrene-d10	19.733	212	8625323	39.366	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.851	264	8941329	46.904	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012806.D
Acq On : 27 Nov 2022 14:01
Operator : CG/JU
Sample : N5683-14
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ESQW7

Manual IntegrationsAPPROVED

Quant Time: Nov 27 23:08:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/28/2022
Supervised By :mohammad ahmed 11/30/2022

