

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP112522\  
 Data File : BP012732.D  
 Acq On : 25 Nov 2022 18:17  
 Operator : CG/JU  
 Sample : PB149034BL  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 SBLK034

Quant Time: Nov 26 06:54:49 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP112522.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Fri Nov 25 15:59:22 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min)      |
|-------------------------------|--------|------|----------|--------|-------|---------------|
| -----                         |        |      |          |        |       |               |
| Internal Standards            |        |      |          |        |       |               |
| 1) 1,4-Dichlorobenzene-d4     | 8.022  | 152  | 482703   | 20.000 | ng/u1 | 0.00          |
| 20) Naphthalene-d8            | 10.840 | 136  | 2129540  | 20.000 | ng/u1 | 0.00          |
| 38) Acenaphthene-d10          | 14.657 | 164  | 1438198  | 20.000 | ng/u1 | 0.00          |
| 64) Phenanthrene-d10          | 17.416 | 188  | 3014815  | 20.000 | ng/u1 | 0.00          |
| 79) Chrysene-d12              | 21.504 | 240  | 2667653  | 20.000 | ng/u1 | 0.00          |
| 88) Perylene-d12              | 24.021 | 264  | 2146408  | 20.000 | ng/u1 | 0.00          |
| System Monitoring Compounds   |        |      |          |        |       |               |
| 3) 1,4-Dioxane-d8             | 3.399  | 96   | 68355    | 6.068  | ng/uL | 0.00          |
| 4) Pyridine-d5                | 3.823  | 84   | 925080   | 27.442 | ng/u1 | 0.00          |
| 7) Phenol-d5                  | 7.169  | 99   | 1144438  | 28.852 | ng/u1 | 0.00          |
| 9) Bis-(2-Chloroethyl)eth...  | 7.346  | 67   | 748668   | 30.631 | ng/u1 | 0.00          |
| 11) 2-Chlorophenol-d4         | 7.552  | 132  | 923133   | 30.543 | ng/u1 | 0.00          |
| 15) 4-Methylphenol-d8         | 8.722  | 113  | 929880   | 29.097 | ng/u1 | 0.00          |
| 21) Nitrobenzene-d5           | 9.193  | 128  | 423004   | 32.454 | ng/u1 | 0.00          |
| 24) 2-Nitrophenol-d4          | 9.916  | 143  | 467676   | 33.793 | ng/u1 | 0.00          |
| 28) 2,4-Dichlorophenol-d3     | 10.452 | 165  | 929274   | 28.777 | ng/u1 | 0.00          |
| 31) 4-Chloroaniline-d4        | 10.975 | 131  | 1338856  | 30.277 | ng/u1 | 0.00          |
| 46) Dimethylphthalate-d6      | 14.063 | 166  | 3254092  | 32.872 | ng/u1 | 0.00          |
| 49) Acenaphthylene-d8         | 14.351 | 160  | 3606228  | 31.221 | ng/u1 | 0.00          |
| 54) 4-Nitrophenol-d4          | 14.834 | 143  | 449282   | 25.456 | ng/u1 | 0.00          |
| 60) Fluorene-d10              | 15.651 | 176  | 2776587  | 32.027 | ng/u1 | 0.00          |
| 65) 4,6-Dinitro-2-methylph... | 15.757 | 200  | 355410   | 24.665 | ng/u1 | 0.00          |
| 73) Anthracene-d10            | 17.516 | 188  | 4479159  | 33.752 | ng/u1 | 0.00          |
| 81) Pyrene-d10                | 19.739 | 212  | 4991563  | 32.202 | ng/u1 | 0.00          |
| 92) Benzo(a)pyrene-d12        | 23.857 | 264  | 3606923  | 34.212 | ng/u1 | 0.00          |
| Target Compounds              |        |      |          |        |       |               |
| 86) Bis(2-ethylhexyl)phtha... | 21.410 | 149  | 5263557  | 73.757 | ng/u1 | Qvalue<br>100 |
| -----                         |        |      |          |        |       |               |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP112522\  
Data File : BP012732.D  
Acq On : 25 Nov 2022 18:17  
Operator : CG/JU  
Sample : PB149034BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
SBLK034

Quant Time: Nov 26 06:54:49 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP112522.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Fri Nov 25 15:59:22 2022  
Response via : Initial Calibration

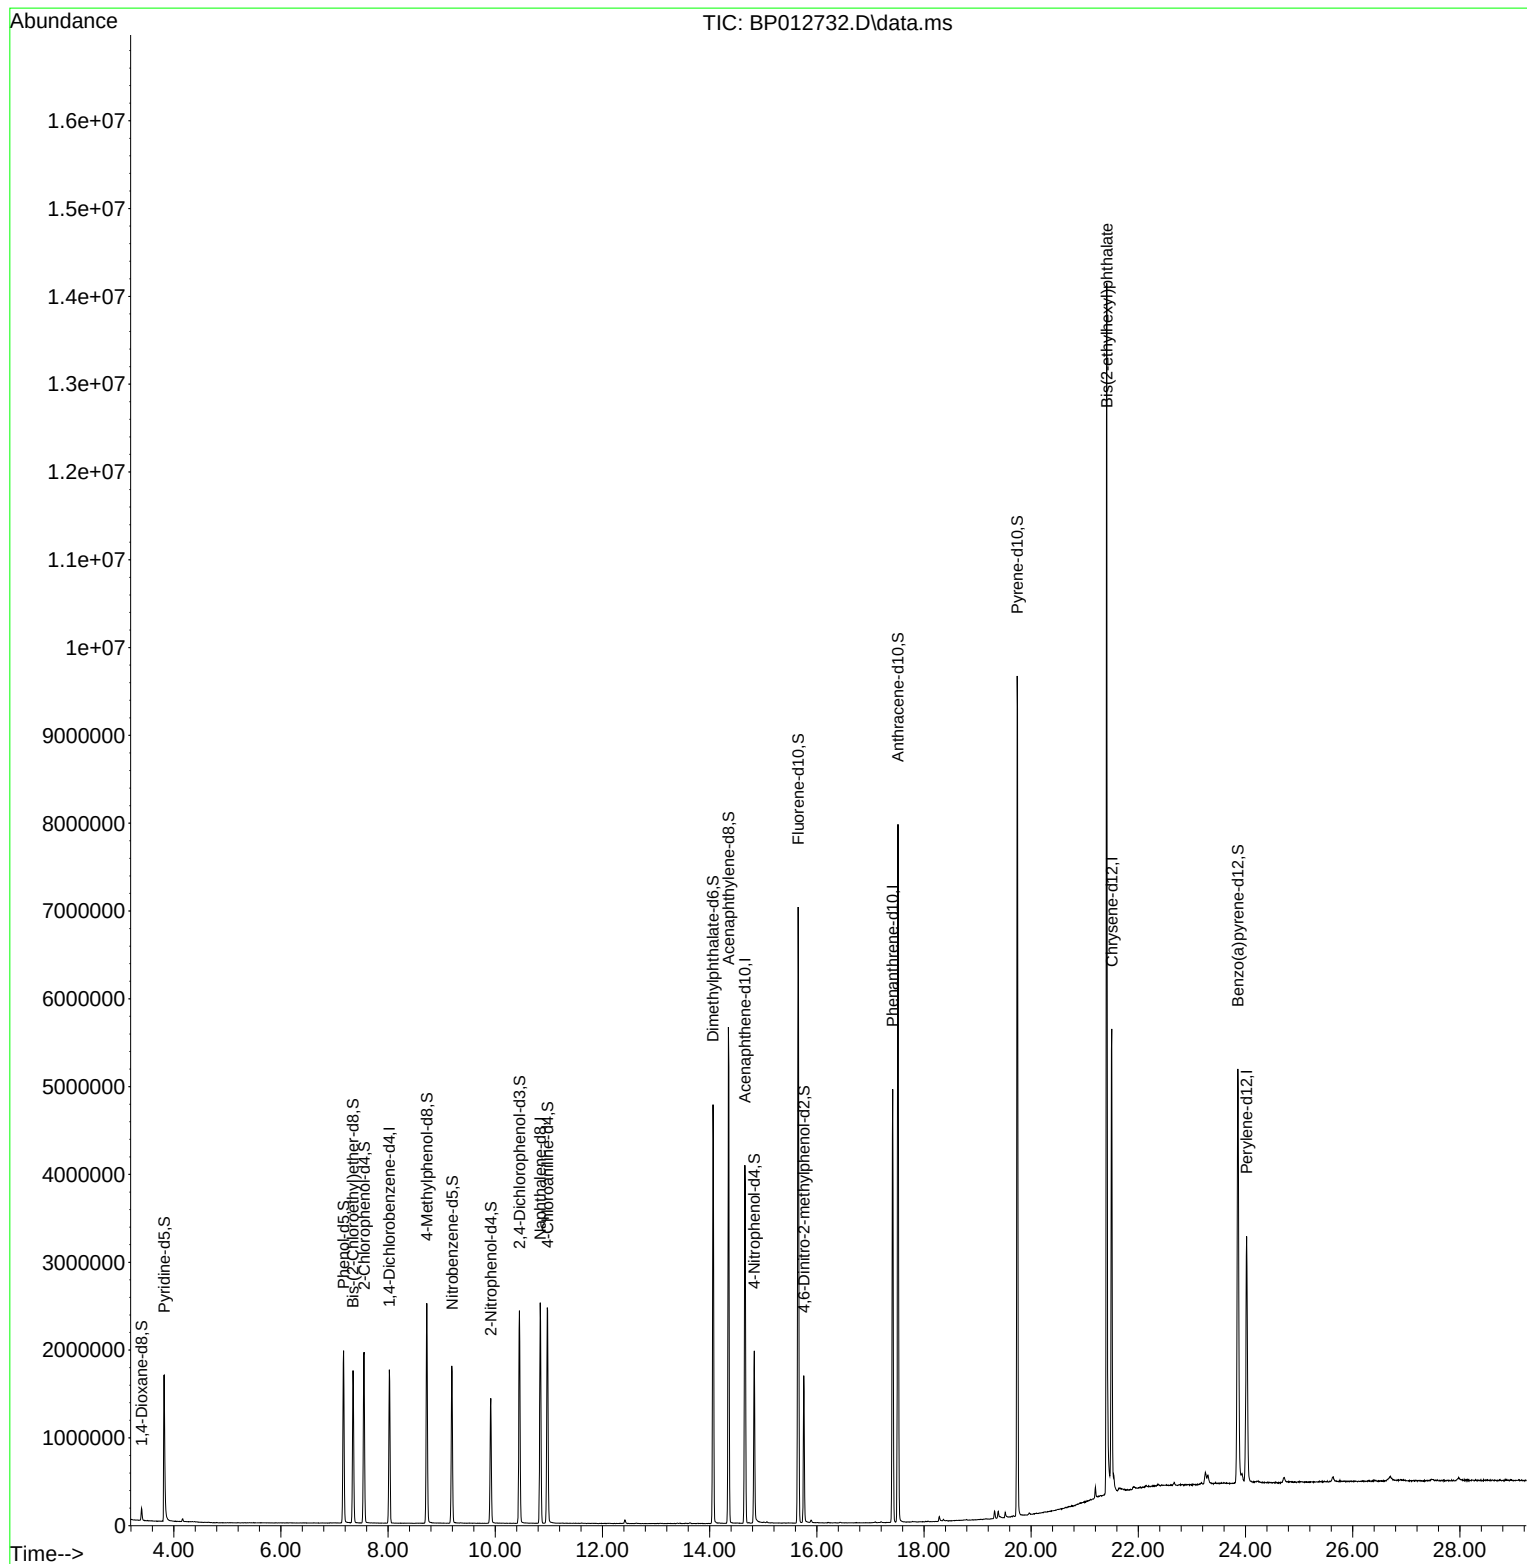

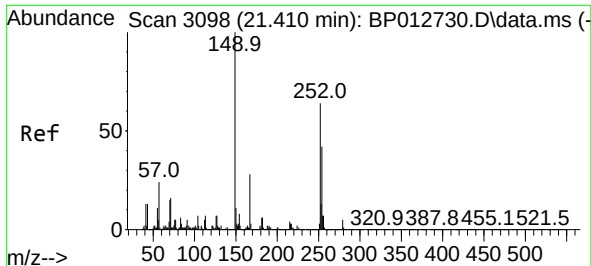

#86  
 Bis(2-ethylhexyl)phthalate  
 Concen: 73.757 ng/ul  
 RT: 21.410 min Scan# 3098  
 Delta R.T. 0.000 min  
 Lab File: BP012732.D  
 Acq: 25 Nov 2022 18:17

Instrument :  
 BNA\_P  
 ClientSampleId :  
 SBLK034

Tgt Ion:149 Resp: 5263557  
 Ion Ratio Lower Upper  
 149 100  
 167 28.6 22.7 34.1  
 279 4.8 3.8 5.6

