

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012734.D
 Acq On : 25 Nov 2022 19:25
 Operator : CG/JU
 Sample : N5592-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AB6

Quant Time: Nov 26 06:59:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 25 15:59:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	509478	20.000	ng/u1	0.00
20) Naphthalene-d8	10.840	136	2281632	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.657	164	1568273	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.416	188	3416394	20.000	ng/u1	0.00
79) Chrysene-d12	21.504	240	2840402	20.000	ng/u1	0.00
88) Perylene-d12	24.021	264	2198320	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	59593	5.012	ng/uL	0.00
4) Pyridine-d5	3.822	84	386106	10.852	ng/u1	0.00
7) Phenol-d5	7.169	99	341020	8.146	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.346	67	882033	34.191	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	867518	27.194	ng/u1	0.00
15) 4-Methylphenol-d8	8.722	113	650915	19.297	ng/u1	0.00
21) Nitrobenzene-d5	9.187	128	535499	38.346	ng/u1	0.00
24) 2-Nitrophenol-d4	9.916	143	553368	37.319	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.451	165	1127193	32.580	ng/u1	0.00
31) 4-Chloroaniline-d4	10.969	131	1237921	26.129	ng/u1	0.00
46) Dimethylphthalate-d6	14.069	166	4456124	41.281	ng/u1	0.00
49) Acenaphthylene-d8	14.351	160	4785758	37.997	ng/u1	0.00
54) 4-Nitrophenol-d4	14.834	143	114749	5.962	ng/u1	0.00
60) Fluorene-d10	15.651	176	3836712	40.584	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	513563	31.452	ng/u1	0.00
73) Anthracene-d10	17.516	188	6286724	41.804	ng/u1	0.00
81) Pyrene-d10	19.745	212	7099365	43.015	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.857	264	4755767	44.043	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.434	88	35476	2.778	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012734.D
Acq On : 25 Nov 2022 19:25
Operator : CG/JU
Sample : N5592-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AB6


Quant Time: Nov 26 06:59:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 25 15:59:22 2022
Response via : Initial Calibration

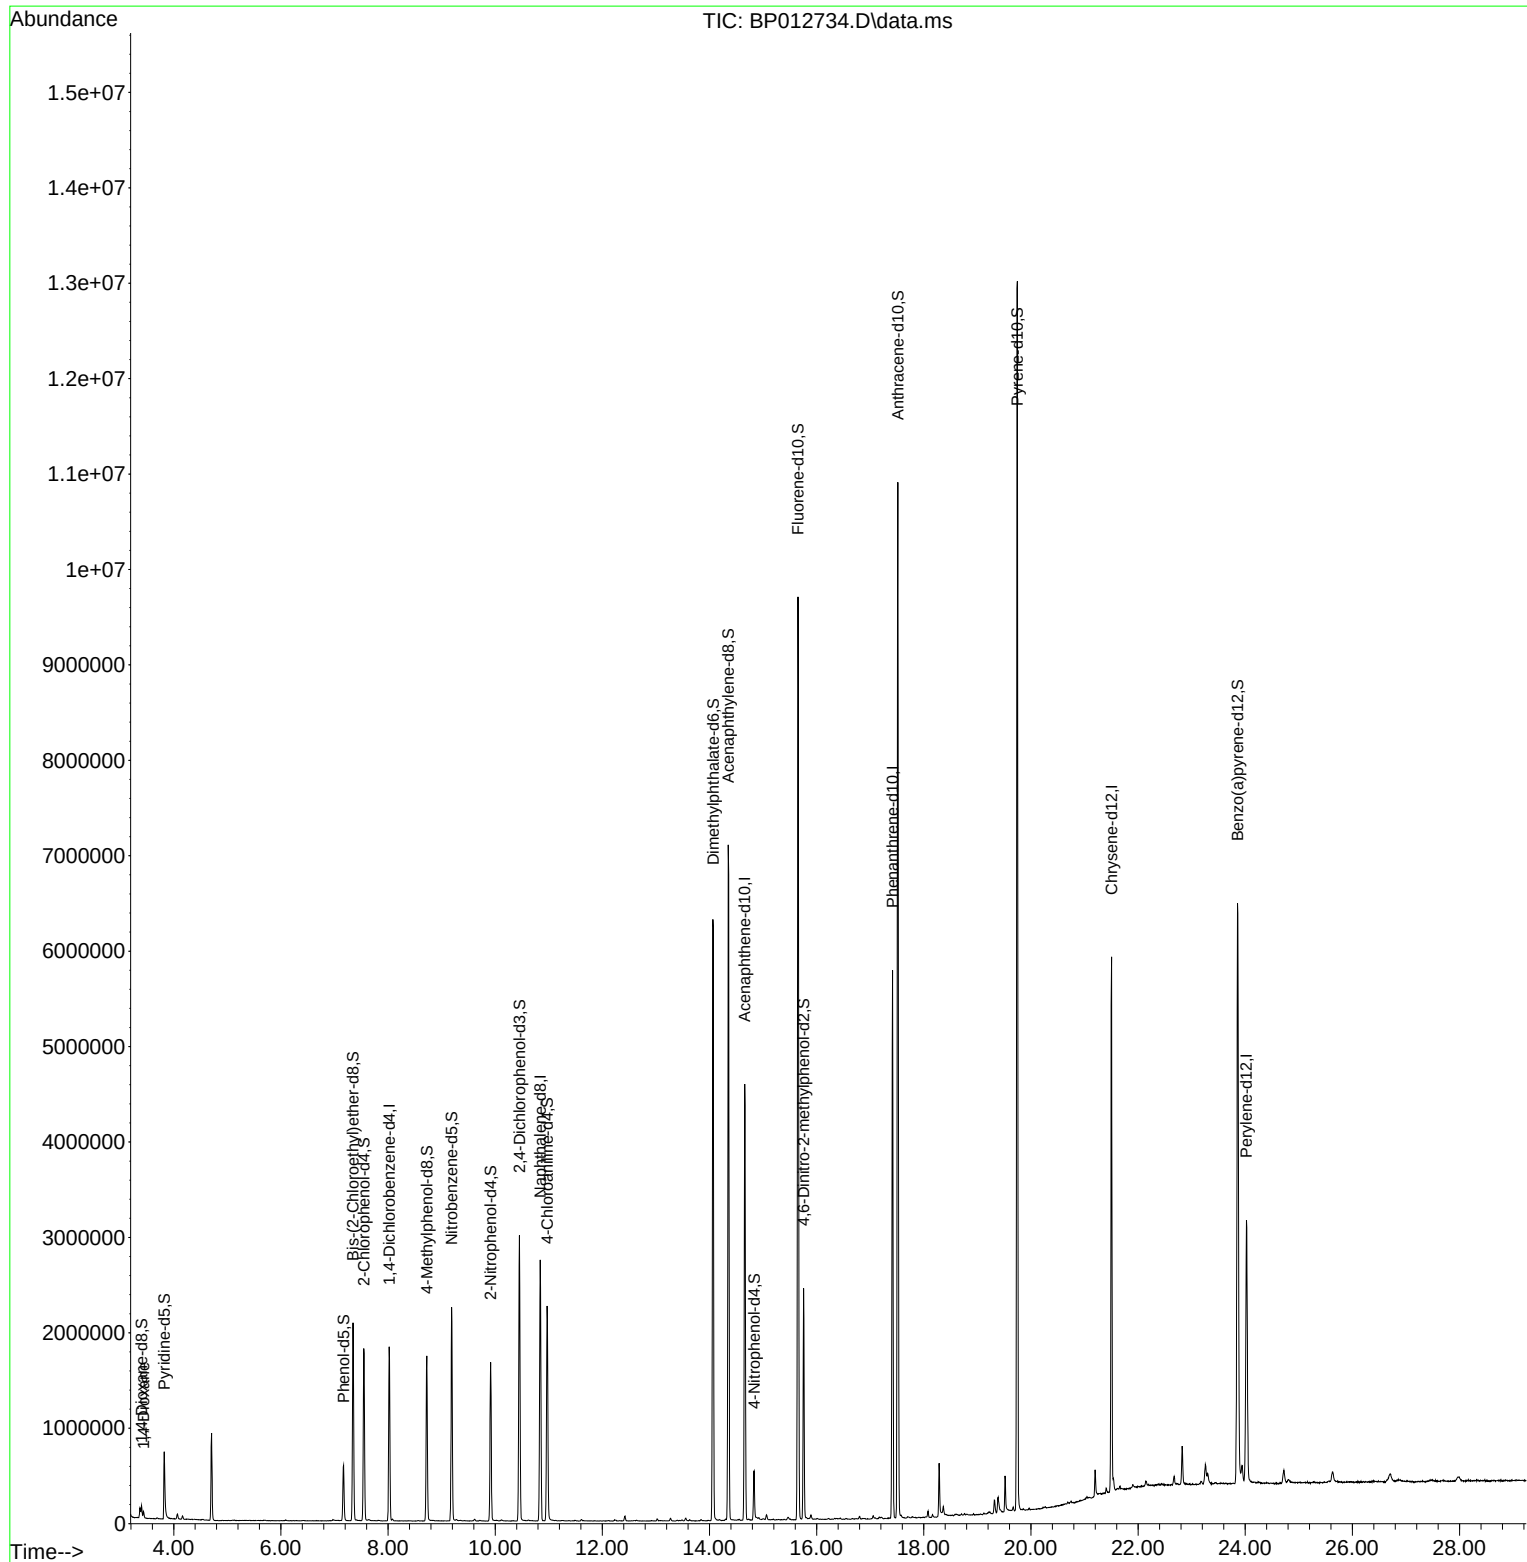

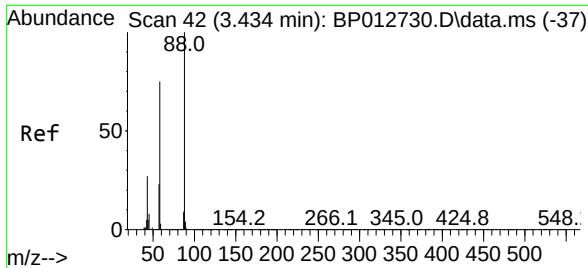

#2
 1,4-Dioxane
 Concen: 2.778 ng/uL
 RT: 3.434 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BP012734.D
 Acq: 25 Nov 2022 19:25

Instrument :
 BNA_P
 ClientSampleId :
 H0AB6

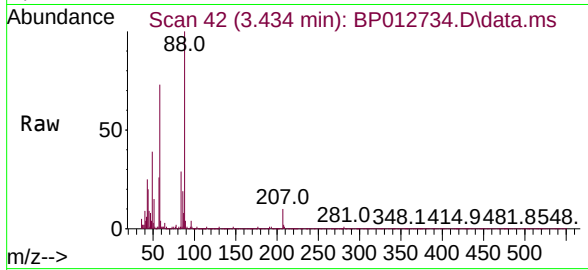

Tgt Ion: 88	Resp: 35476
Ion Ratio	Lower Upper
88	100
43	24.5 22.6 34.0
58	73.3 59.6 89.4

