

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012735.D
 Acq On : 25 Nov 2022 19:59
 Operator : CG/JU
 Sample : N5592-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AB7

Quant Time: Nov 26 07:02:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 25 15:59:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	486997	20.000	ng/u1	0.00
20) Naphthalene-d8	10.840	136	2165864	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.657	164	1453594	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.416	188	2967437	20.000	ng/u1	0.00
79) Chrysene-d12	21.498	240	1971099	20.000	ng/u1	0.00
88) Perylene-d12	24.021	264	1602286	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	53959	4.748	ng/uL	0.00
4) Pyridine-d5	3.822	84	335449	9.863	ng/u1	0.00
7) Phenol-d5	7.169	99	274273	6.854	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.346	67	779160	31.598	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	753699	24.717	ng/u1	0.00
15) 4-Methylphenol-d8	8.722	113	523440	16.234	ng/u1	0.00
21) Nitrobenzene-d5	9.187	128	457875	34.540	ng/u1	0.00
24) 2-Nitrophenol-d4	9.916	143	472224	33.549	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.451	165	922645	28.093	ng/u1	0.00
31) 4-Chloroaniline-d4	10.969	131	1138299	25.310	ng/u1	0.00
46) Dimethylphthalate-d6	14.063	166	3450663	34.488	ng/u1	0.00
49) Acenaphthylene-d8	14.351	160	3848905	32.969	ng/u1	0.00
54) 4-Nitrophenol-d4	14.834	143	66934	3.752	ng/u1	0.00
60) Fluorene-d10	15.651	176	3016849	34.430	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	355322	25.053	ng/u1	0.00
73) Anthracene-d10	17.516	188	4842618	37.073	ng/u1	0.00
81) Pyrene-d10	19.739	212	4965561	43.355	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.857	264	2963682	37.657	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.440	88	31002	2.540 ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012735.D
Acq On : 25 Nov 2022 19:59
Operator : CG/JU
Sample : N5592-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AB7


Quant Time: Nov 26 07:02:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 25 15:59:22 2022
Response via : Initial Calibration

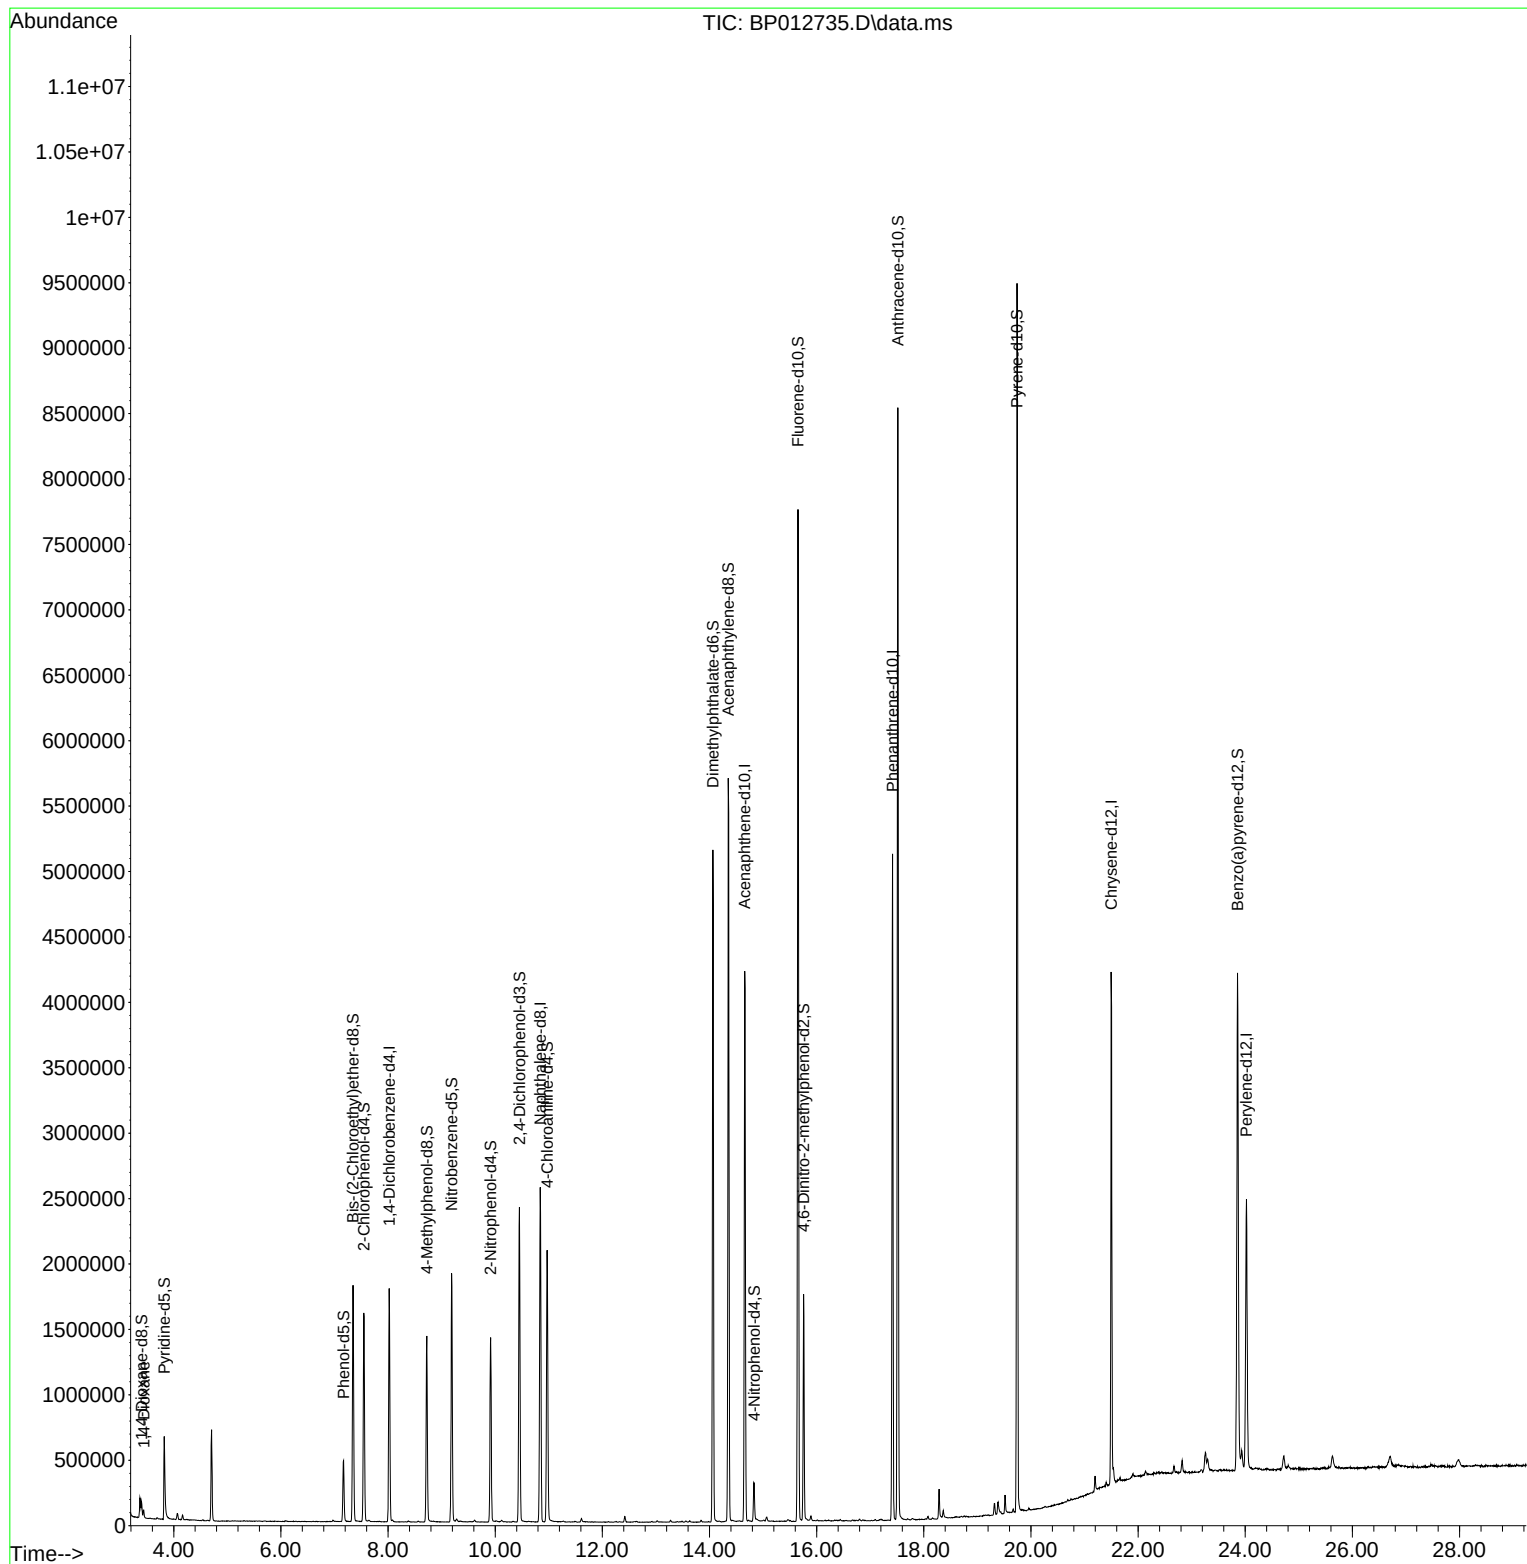

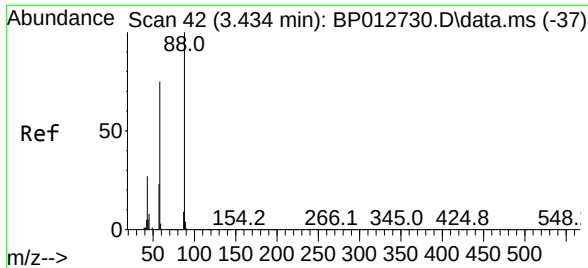

#2
 1,4-Dioxane
 Concen: 2.540 ng/uL
 RT: 3.440 min Scan# 43
 Delta R.T. 0.006 min
 Lab File: BP012735.D
 Acq: 25 Nov 2022 19:59

Instrument :
 BNA_P
 ClientSampleId :
 H0AB7

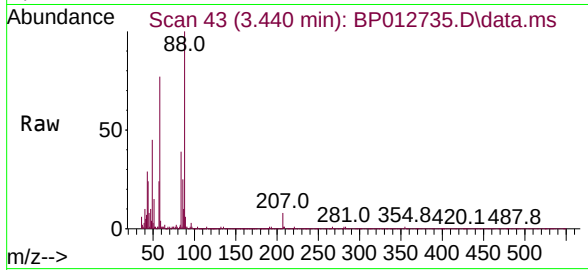

Tgt Ion:	88	Resp:	31002
Ion	Ratio	Lower	Upper
88	100		
43	29.1	22.6	34.0
58	77.3	59.6	89.4

