

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012737.D
 Acq On : 25 Nov 2022 21:07
 Operator : CG/JU
 Sample : N5592-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AB9

Quant Time: Nov 26 07:06:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 25 15:59:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	518730	20.000	ng/u1	0.00
20) Naphthalene-d8	10.840	136	2296982	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.657	164	1539157	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.416	188	3193755	20.000	ng/u1	0.00
79) Chrysene-d12	21.498	240	2366489	20.000	ng/u1	0.00
88) Perylene-d12	24.021	264	1803006	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	68521	5.660	ng/uL	0.00
4) Pyridine-d5	3.822	84	429859	11.866	ng/u1	0.00
7) Phenol-d5	7.169	99	390468	9.160	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.346	67	963057	36.666	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	968173	29.808	ng/u1	0.00
15) 4-Methylphenol-d8	8.722	113	695949	20.264	ng/u1	0.00
21) Nitrobenzene-d5	9.187	128	565460	40.221	ng/u1	0.00
24) 2-Nitrophenol-d4	9.916	143	604950	40.525	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.452	165	1155823	33.184	ng/u1	0.00
31) 4-Chloroaniline-d4	10.969	131	1434597	30.078	ng/u1	0.00
46) Dimethylphthalate-d6	14.063	166	4099221	38.693	ng/u1	0.00
49) Acenaphthylene-d8	14.351	160	4601938	37.228	ng/u1	0.00
54) 4-Nitrophenol-d4	14.834	143	104408	5.528	ng/u1	0.00
60) Fluorene-d10	15.651	176	3566857	38.444	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	458296	30.024	ng/u1	0.00
73) Anthracene-d10	17.516	188	5724908	40.722	ng/u1	0.00
81) Pyrene-d10	19.739	212	6196171	45.061	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.857	264	3756325	42.415	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.440	88	45055	3.466	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012737.D
Acq On : 25 Nov 2022 21:07
Operator : CG/JU
Sample : N5592-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AB9


Quant Time: Nov 26 07:06:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 25 15:59:22 2022
Response via : Initial Calibration

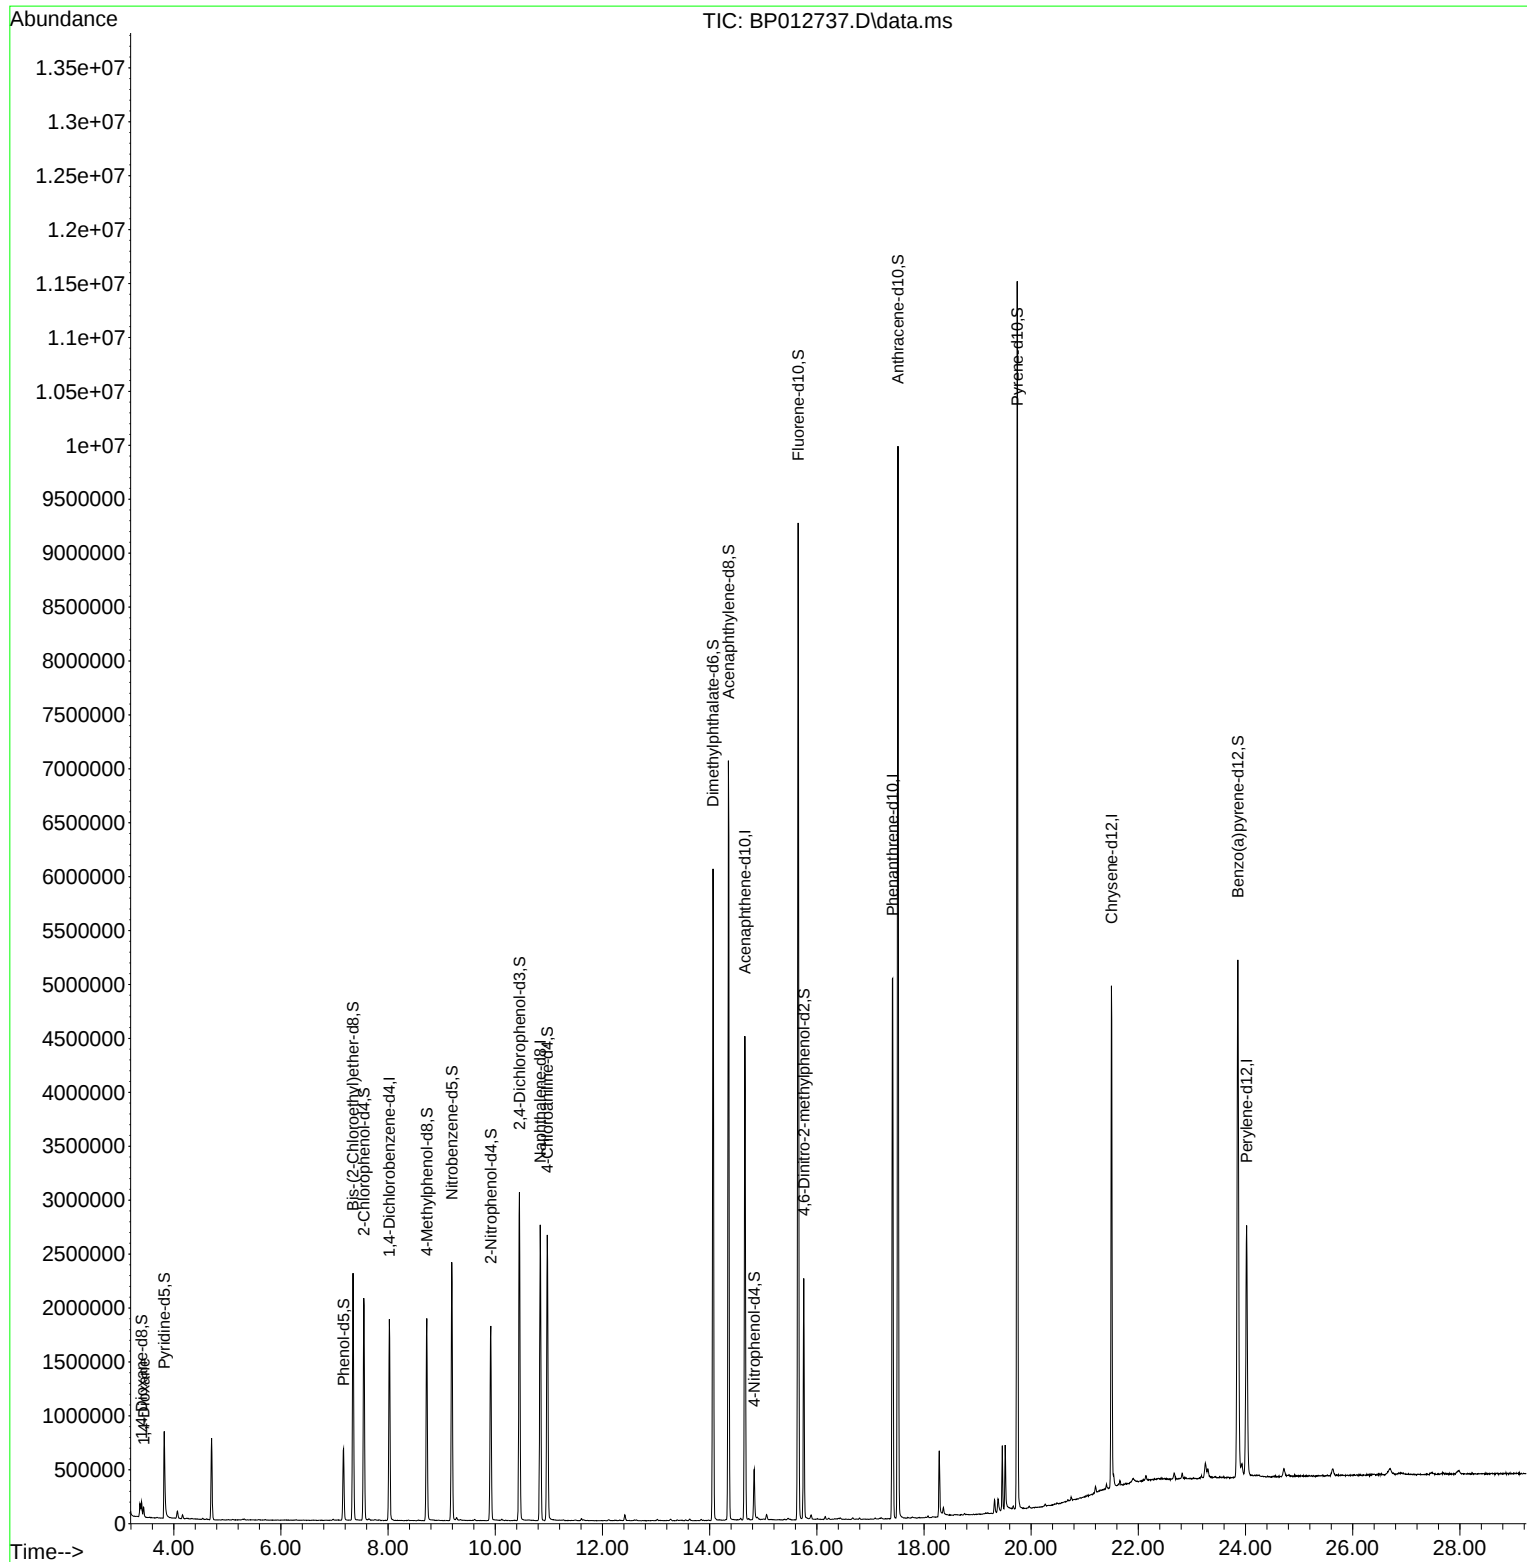

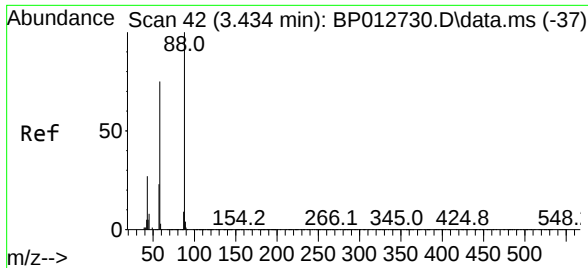

#2
 1,4-Dioxane
 Concen: 3.466 ng/uL
 RT: 3.440 min Scan# 43
 Delta R.T. 0.006 min
 Lab File: BP012737.D
 Acq: 25 Nov 2022 21:07

Instrument :
 BNA_P
 ClientSampleId :
 H0AB9

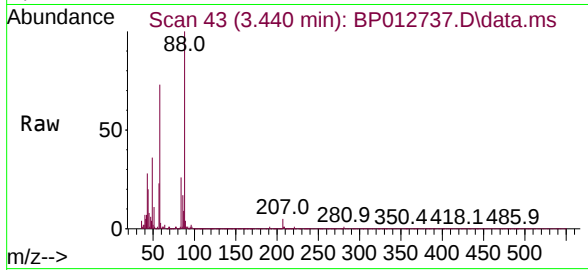

Tgt Ion:	88	Resp:	45055
Ion	Ratio	Lower	Upper
88	100		
43	27.9	22.6	34.0
58	73.0	59.6	89.4

