

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012738.D
 Acq On : 25 Nov 2022 21:41
 Operator : CG/JU
 Sample : N5592-15
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC0

Quant Time: Nov 26 07:08:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 25 15:59:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	502922	20.000	ng/u1	0.00
20) Naphthalene-d8	10.840	136	2256211	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.657	164	1515647	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.416	188	3157201	20.000	ng/u1	0.00
79) Chrysene-d12	21.498	240	2245718	20.000	ng/u1	0.00
88) Perylene-d12	24.015	264	1705219	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	56334	4.800	ng/uL	0.00
4) Pyridine-d5	3.822	84	338357	9.634	ng/u1	0.00
7) Phenol-d5	7.163	99	310921	7.524	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.346	67	876240	34.409	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	852953	27.086	ng/u1	0.00
15) 4-Methylphenol-d8	8.722	113	593870	17.836	ng/u1	0.00
21) Nitrobenzene-d5	9.187	128	511631	37.050	ng/u1	0.00
24) 2-Nitrophenol-d4	9.916	143	541244	36.913	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.451	165	1045849	30.569	ng/u1	0.00
31) 4-Chloroaniline-d4	10.969	131	1340358	28.610	ng/u1	0.00
46) Dimethylphthalate-d6	14.063	166	3974001	38.093	ng/u1	0.00
49) Acenaphthylene-d8	14.351	160	4289617	35.240	ng/u1	0.00
54) 4-Nitrophenol-d4	14.834	143	85417	4.592	ng/u1	0.00
60) Fluorene-d10	15.651	176	3405774	37.277	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	438589	29.065	ng/u1	0.00
73) Anthracene-d10	17.516	188	5662751	40.746	ng/u1	0.00
81) Pyrene-d10	19.739	212	6055703	46.408	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.857	264	3537278	42.232	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.434	88	38933	3.089	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012738.D
Acq On : 25 Nov 2022 21:41
Operator : CG/JU
Sample : N5592-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC0


Quant Time: Nov 26 07:08:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 25 15:59:22 2022
Response via : Initial Calibration

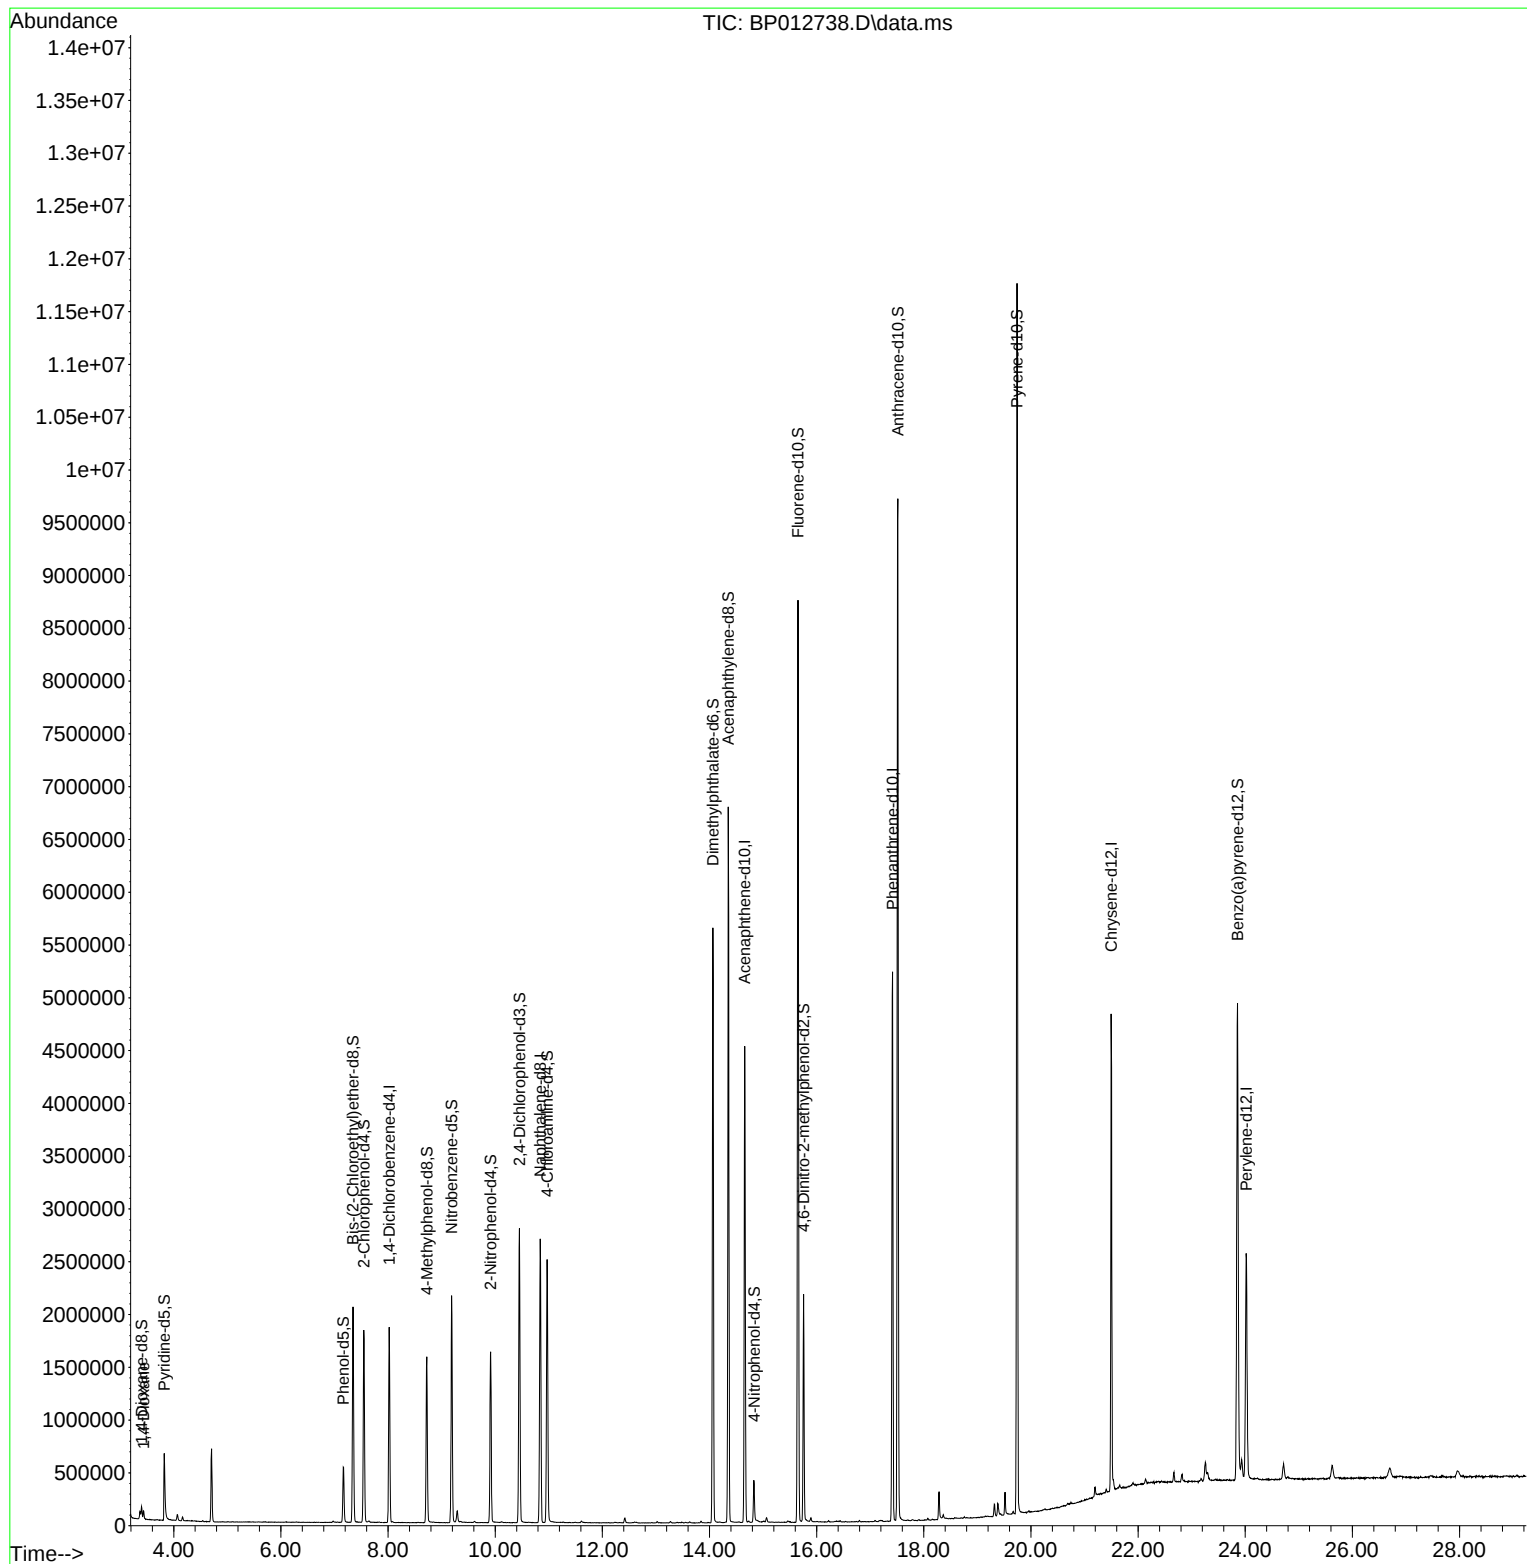

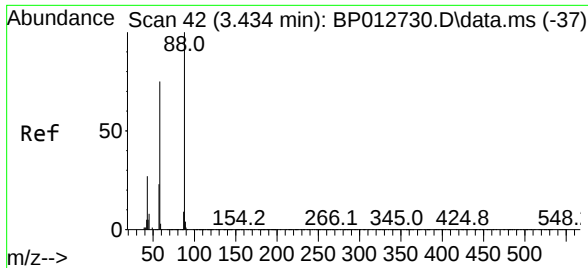

#2
 1,4-Dioxane
 Concen: 3.089 ng/uL
 RT: 3.434 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BP012738.D
 Acq: 25 Nov 2022 21:41

Instrument :
 BNA_P
 ClientSampleId :
 H0AC0

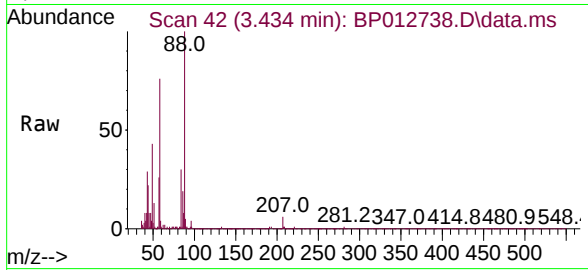

Tgt Ion: 88 Resp: 38933

Ion	Ratio	Lower	Upper
88	100		
43	29.0	22.6	34.0
58	76.2	59.6	89.4

