

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012740.D
 Acq On : 25 Nov 2022 22:49
 Operator : CG/JU
 Sample : N5592-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC2

Quant Time: Nov 26 07:12:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 25 15:59:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	589456	20.000	ng/u1	0.00
20) Naphthalene-d8	10.840	136	2686729	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.657	164	1892275	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.416	188	4187673	20.000	ng/u1	0.00
79) Chrysene-d12	21.498	240	3930755	20.000	ng/u1	0.00
88) Perylene-d12	24.021	264	3417445	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	56532	4.110	ng/uL	0.00
4) Pyridine-d5	3.823	84	304898	7.407	ng/u1	0.00
7) Phenol-d5	7.164	99	283843	5.860	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.346	67	831523	27.860	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	785148	21.273	ng/u1	0.00
15) 4-Methylphenol-d8	8.722	113	536680	13.752	ng/u1	0.00
21) Nitrobenzene-d5	9.187	128	488621	29.714	ng/u1	0.00
24) 2-Nitrophenol-d4	9.910	143	491105	28.126	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.452	165	959667	23.555	ng/u1	0.00
31) 4-Chloroaniline-d4	10.969	131	1276148	22.874	ng/u1	0.00
46) Dimethylphthalate-d6	14.063	166	4200384	32.249	ng/u1	0.00
49) Acenaphthylene-d8	14.351	160	4343427	28.580	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	97901	4.216	ng/u1	-0.01
60) Fluorene-d10	15.651	176	3679957	32.261	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	485295	24.247	ng/u1	0.00
73) Anthracene-d10	17.516	188	6306636	34.212	ng/u1	0.00
81) Pyrene-d10	19.739	212	7381779	32.320	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.857	264	5950824	35.451	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.434	88	47200	3.195	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012740.D
Acq On : 25 Nov 2022 22:49
Operator : CG/JU
Sample : N5592-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC2


Quant Time: Nov 26 07:12:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 25 15:59:22 2022
Response via : Initial Calibration

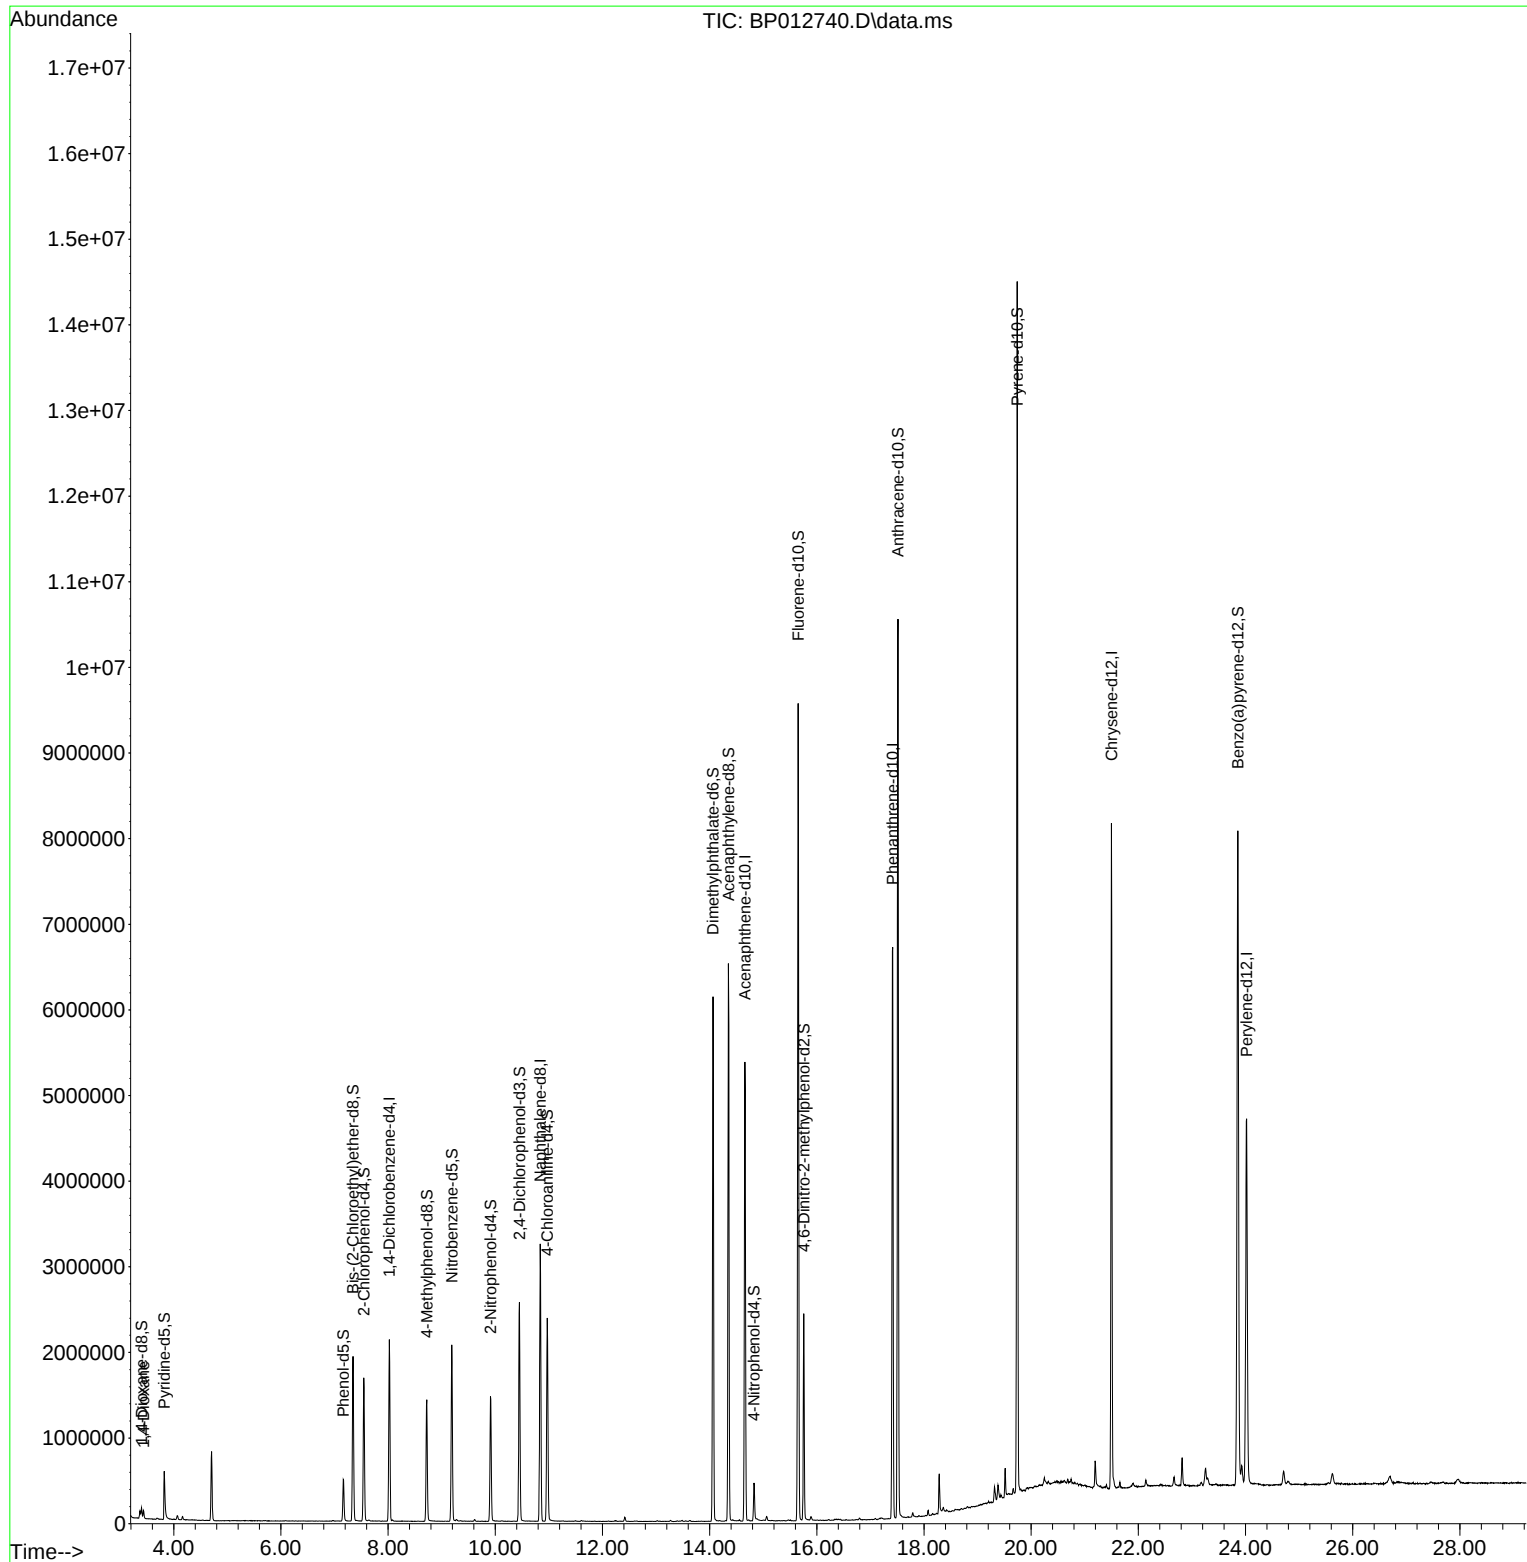

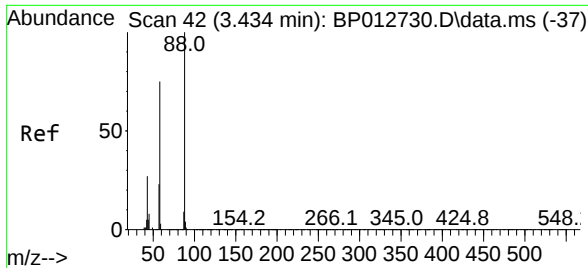

#2
 1,4-Dioxane
 Concen: 3.195 ng/uL
 RT: 3.434 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BP012740.D
 Acq: 25 Nov 2022 22:49

Instrument :
 BNA_P
 ClientSampleId :
 H0AC2

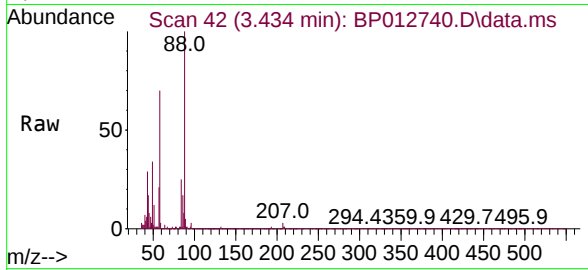

Tgt Ion:	88	Resp:	47200
Ion	Ratio	Lower	Upper
88	100		
43	29.1	22.6	34.0
58	70.2	59.6	89.4

