

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012741.D
 Acq On : 25 Nov 2022 23:24
 Operator : CG/JU
 Sample : N5592-18
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC3

Quant Time: Nov 26 07:14:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 25 15:59:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	515518	20.000	ng/u1	0.00
20) Naphthalene-d8	10.840	136	2310978	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.657	164	1574690	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.416	188	3352721	20.000	ng/u1	0.00
79) Chrysene-d12	21.498	240	2712672	20.000	ng/u1	0.00
88) Perylene-d12	24.015	264	2078226	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	53996	4.488	ng/uL	0.00
4) Pyridine-d5	3.822	84	374610	10.405	ng/u1	0.00
7) Phenol-d5	7.169	99	289925	6.844	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.346	67	935462	35.837	ng/u1	0.00
11) 2-Chlorophenol-d4	7.552	132	856630	26.539	ng/u1	0.00
15) 4-Methylphenol-d8	8.722	113	578818	16.959	ng/u1	0.00
21) Nitrobenzene-d5	9.187	128	559381	39.548	ng/u1	0.00
24) 2-Nitrophenol-d4	9.916	143	561966	37.418	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.451	165	1073675	30.639	ng/u1	0.00
31) 4-Chloroaniline-d4	10.969	131	1415204	29.491	ng/u1	0.00
46) Dimethylphthalate-d6	14.063	166	4213332	38.872	ng/u1	0.00
49) Acenaphthylene-d8	14.351	160	4681823	37.020	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	78986	4.087	ng/u1	-0.01
60) Fluorene-d10	15.651	176	3655872	38.514	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	465271	29.035	ng/u1	0.00
73) Anthracene-d10	17.510	188	6146825	41.650	ng/u1	0.00
81) Pyrene-d10	19.739	212	6836123	43.371	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.857	264	4427713	43.375	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.434	88	44358	3.433	ng/uL	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012741.D
Acq On : 25 Nov 2022 23:24
Operator : CG/JU
Sample : N5592-18
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC3


Quant Time: Nov 26 07:14:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 25 15:59:22 2022
Response via : Initial Calibration

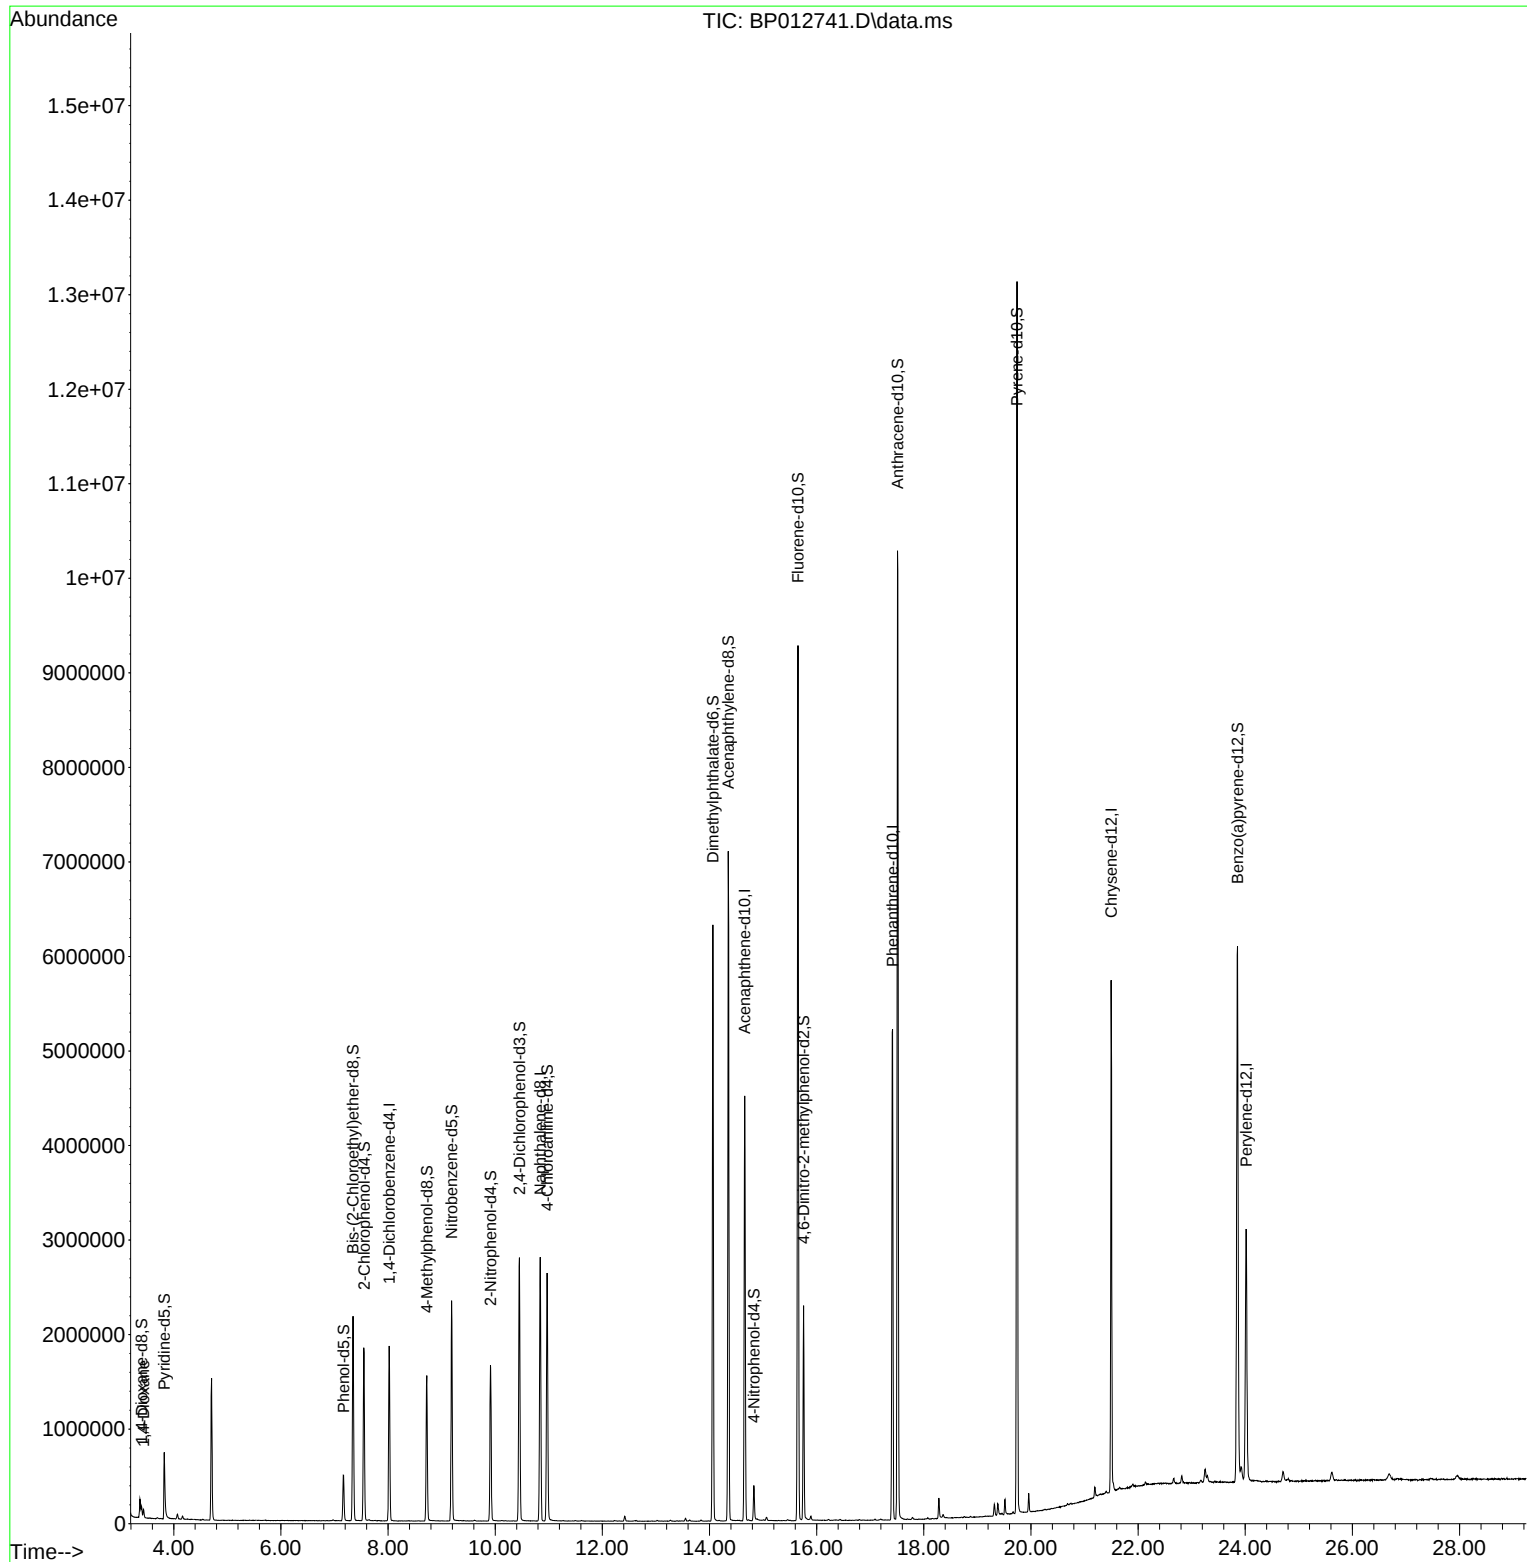

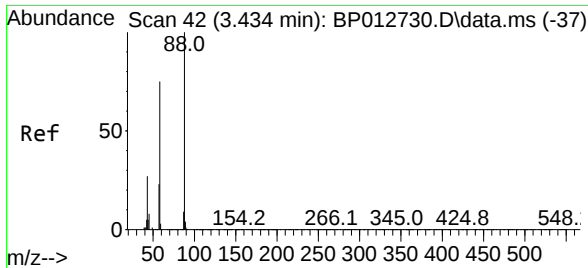

#2
 1,4-Dioxane
 Concen: 3.433 ng/uL
 RT: 3.434 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BP012741.D
 Acq: 25 Nov 2022 23:24

Instrument :
 BNA_P
 ClientSampleId :
 H0AC3

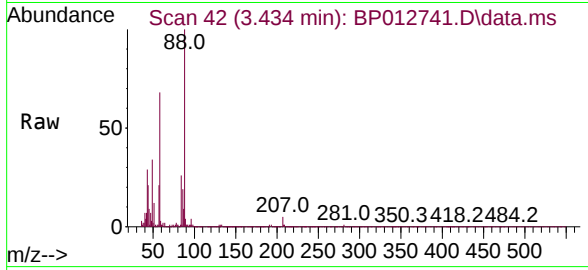

Tgt Ion:	88	Resp:	44358
Ion	Ratio	Lower	Upper
88	100		
43	29.2	22.6	34.0
58	68.0	59.6	89.4

