

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012742.D
 Acq On : 25 Nov 2022 23:58
 Operator : CG/JU
 Sample : N5592-19
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC4

Quant Time: Nov 26 07:16:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 25 15:59:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	493944	20.000	ng/u1	0.00
20) Naphthalene-d8	10.840	136	2181556	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.657	164	1440643	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.416	188	2954477	20.000	ng/u1	0.00
79) Chrysene-d12	21.498	240	1986929	20.000	ng/u1	0.00
88) Perylene-d12	24.015	264	1540646	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	54895	4.762	ng/uL	0.00
4) Pyridine-d5	3.822	84	345804	10.025	ng/u1	0.00
7) Phenol-d5	7.163	99	297909	7.340	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.346	67	923358	36.919	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	887531	28.697	ng/u1	0.00
15) 4-Methylphenol-d8	8.722	113	587372	17.961	ng/u1	0.00
21) Nitrobenzene-d5	9.187	128	543059	40.671	ng/u1	0.00
24) 2-Nitrophenol-d4	9.910	143	568344	40.087	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.451	165	1083358	32.749	ng/u1	0.00
31) 4-Chloroaniline-d4	10.969	131	1365261	30.138	ng/u1	0.00
46) Dimethylphthalate-d6	14.063	166	3894628	39.275	ng/u1	0.00
49) Acenaphthylene-d8	14.351	160	4434940	38.331	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	72044	4.075	ng/u1	-0.01
60) Fluorene-d10	15.651	176	3392869	39.069	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	411884	29.168	ng/u1	0.00
73) Anthracene-d10	17.510	188	5435859	41.797	ng/u1	0.00
81) Pyrene-d10	19.739	212	5712260	49.477	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.851	264	3257017	43.039	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.434	88	48057	3.882	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012742.D
Acq On : 25 Nov 2022 23:58
Operator : CG/JU
Sample : N5592-19
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC4

Quant Time: Nov 26 07:16:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 25 15:59:22 2022
Response via : Initial Calibration

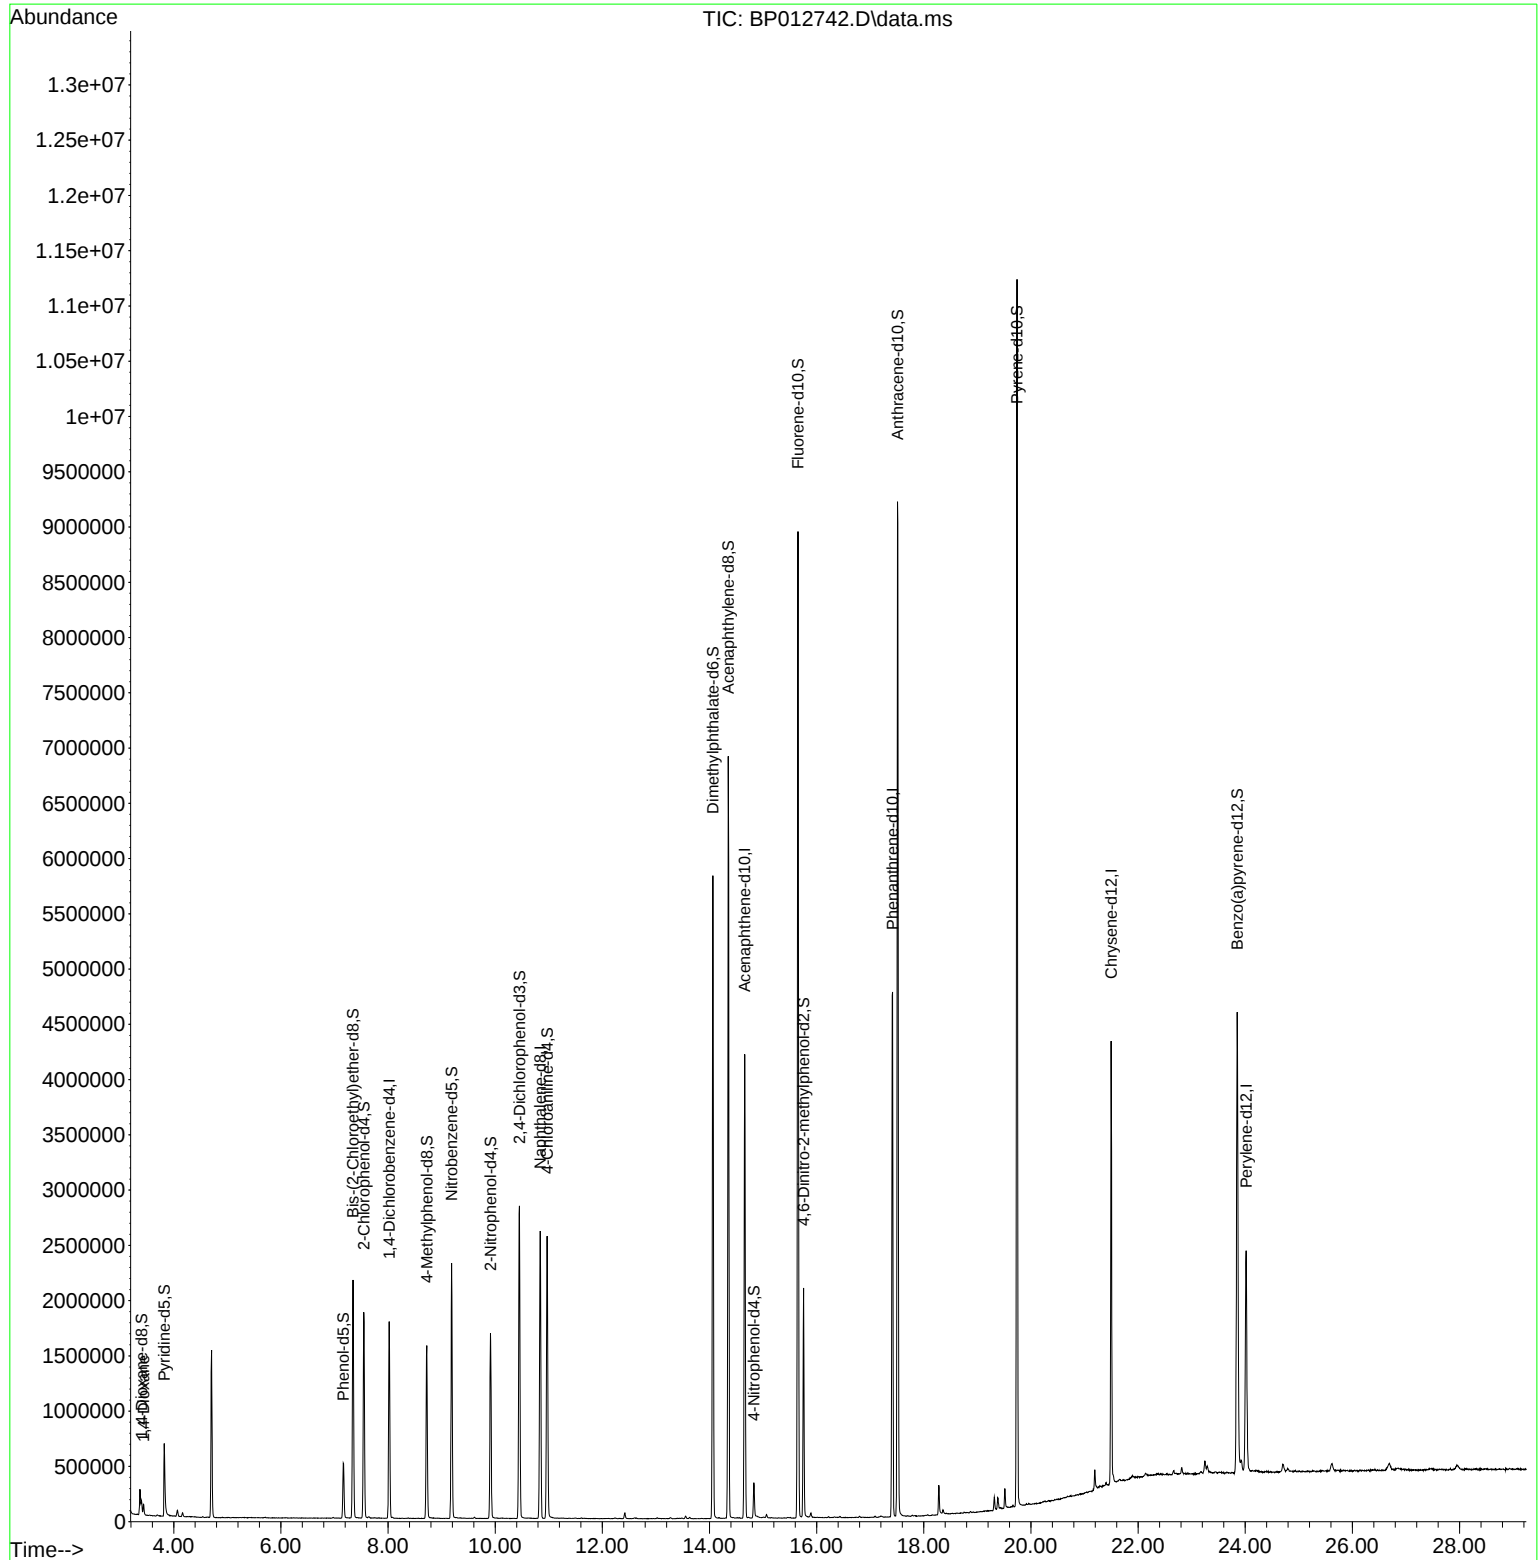

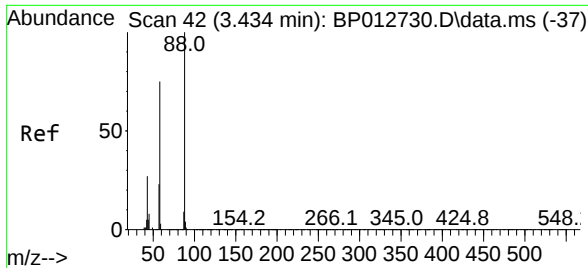

#2
 1,4-Dioxane
 Concen: 3.882 ng/uL
 RT: 3.434 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BP012742.D
 Acq: 25 Nov 2022 23:58

Instrument :
 BNA_P
 ClientSampleId :
 H0AC4

Tgt Ion: 88	Resp: 48057
Ion Ratio	Lower Upper
88	100
43	29.2 22.6 34.0
58	72.8 59.6 89.4

