

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012744.D
 Acq On : 26 Nov 2022 01:06
 Operator : CG/JU
 Sample : N5592-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA3

Quant Time: Nov 26 07:20:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 25 15:59:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	548483	20.000	ng/u1	0.00
20) Naphthalene-d8	10.840	136	2465665	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.657	164	1636201	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.410	188	3333892	20.000	ng/u1	0.00
79) Chrysene-d12	21.498	240	2174755	20.000	ng/u1	0.00
88) Perylene-d12	24.015	264	1708939	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	61166	4.779	ng/uL	0.00
4) Pyridine-d5	3.822	84	307326	8.023	ng/u1	0.00
7) Phenol-d5	7.163	99	307640	6.826	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.346	67	855373	30.800	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	809303	23.565	ng/u1	0.00
15) 4-Methylphenol-d8	8.722	113	587267	16.172	ng/u1	0.00
21) Nitrobenzene-d5	9.187	128	509502	33.761	ng/u1	0.00
24) 2-Nitrophenol-d4	9.910	143	502283	31.346	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.451	165	1040885	27.840	ng/u1	0.00
31) 4-Chloroaniline-d4	10.969	131	1035499	20.225	ng/u1	0.00
46) Dimethylphthalate-d6	14.063	166	4180863	37.123	ng/u1	0.00
49) Acenaphthylene-d8	14.351	160	4496378	34.217	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	78353	3.902	ng/u1	-0.01
60) Fluorene-d10	15.651	176	3551599	36.009	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	404107	25.361	ng/u1	0.00
73) Anthracene-d10	17.510	188	5718093	38.964	ng/u1	0.00
81) Pyrene-d10	19.739	212	5914300	46.803	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.851	264	3341876	39.812	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.440	88	14763	1.074 ng/uL	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012744.D
Acq On : 26 Nov 2022 01:06
Operator : CG/JU
Sample : N5592-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA3


Quant Time: Nov 26 07:20:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 25 15:59:22 2022
Response via : Initial Calibration

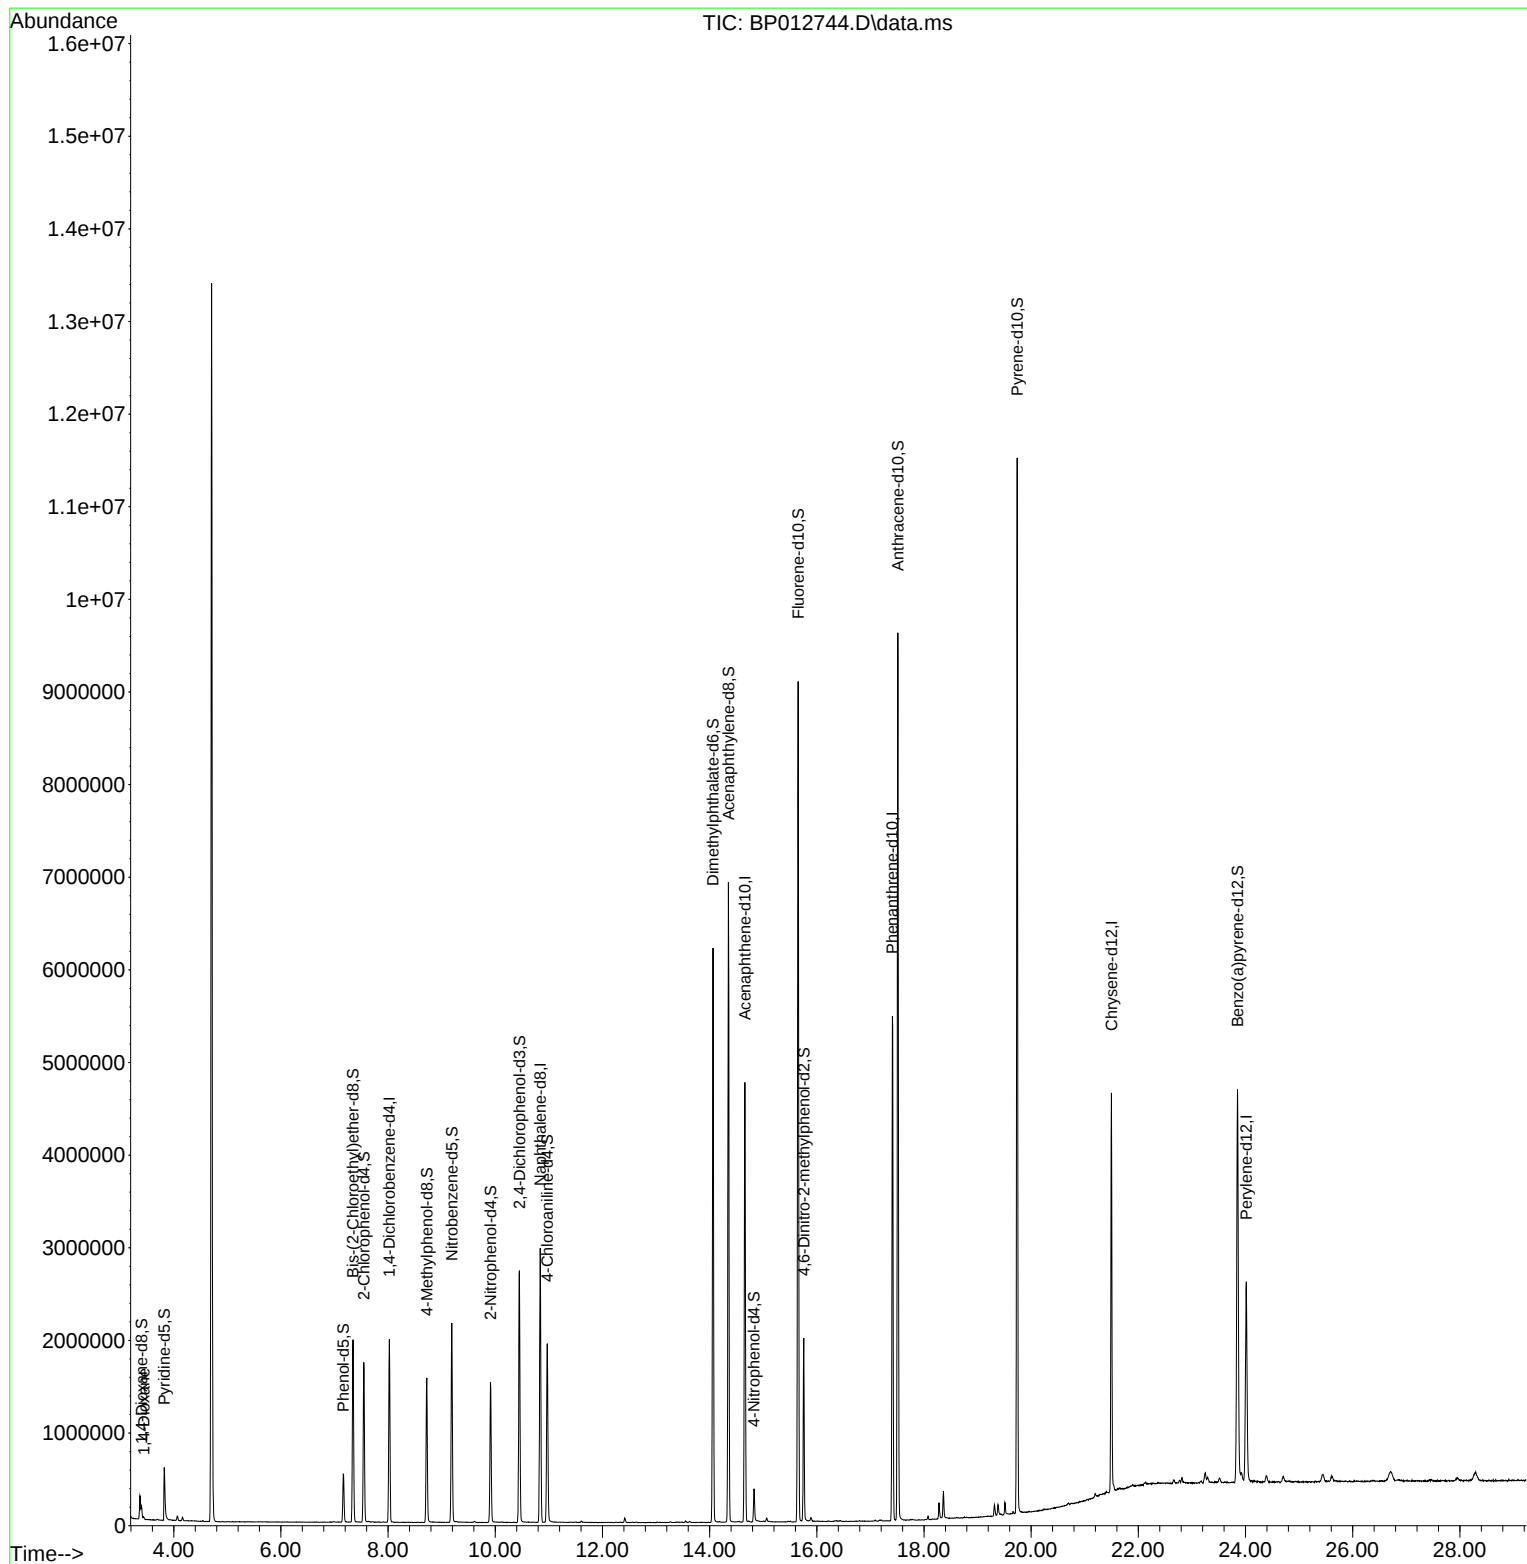

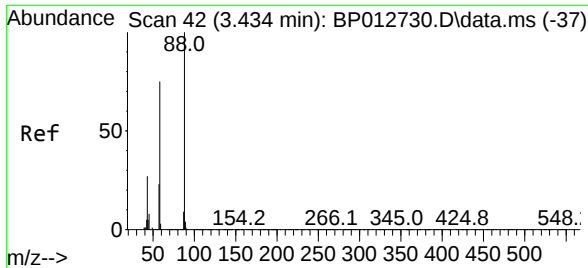

#2
 1,4-Dioxane
 Concen: 1.074 ng/uL
 RT: 3.440 min Scan# 43
 Delta R.T. 0.006 min
 Lab File: BP012744.D
 Acq: 26 Nov 2022 01:06

Instrument :
 BNA_P
 ClientSampleId :
 H0AA3

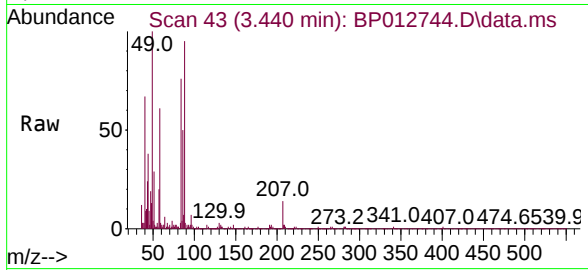

Tgt Ion: 88	Resp: 14763
Ion Ratio	Lower Upper
88	100
43	25.8 22.6 34.0
58	64.2 59.6 89.4

