

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012765.D
 Acq On : 26 Nov 2022 13:36
 Operator : CG/JU
 Sample : N5592-05DL 10X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AB0DL

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/28/2022
 Supervised By :mohammad ahmed 11/30/2022

Quant Time: Nov 27 21:51:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 25 15:59:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	511529	20.000	ng/u1	0.00
20) Naphthalene-d8	10.834	136	2232558	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.657	164	1562920	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.410	188	3433828	20.000	ng/u1	0.00
79) Chrysene-d12	21.492	240	2829351	20.000	ng/u1	-0.01
88) Perylene-d12	24.010	264	2202474	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	4778m	0.400	ng/uL	0.00
4) Pyridine-d5	3.840	84	31849m	0.892	ng/u1	0.02
7) Phenol-d5	7.163	99	26380	0.628	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	68351	2.639	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	61855	1.931	ng/u1	0.00
15) 4-Methylphenol-d8	8.722	113	43812	1.294	ng/u1	0.00
21) Nitrobenzene-d5	9.181	128	27525	2.014	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.910	143	26405	1.820	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.452	165	71717	2.118	ng/u1	0.00
31) 4-Chloroaniline-d4	10.969	131	63459	1.369	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	363811	3.382	ng/u1	-0.01
49) Acenaphthylene-d8	14.351	160	325259	2.591	ng/u1	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	0.00
60) Fluorene-d10	15.645	176	317187	3.367	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/u1	0.00
73) Anthracene-d10	17.510	188	539224	3.567	ng/u1	0.00
81) Pyrene-d10	19.733	212	612222	3.724	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.845	264	339242	3.136	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.434	88	156156	12.180	ng/uL	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012765.D
Acq On : 26 Nov 2022 13:36
Operator : CG/JU
Sample : N5592-05DL 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
H0AB0DL

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/28/2022
Supervised By :mohammad ahmed 11/30/2022


Quant Time: Nov 27 21:51:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 25 15:59:22 2022
Response via : Initial Calibration

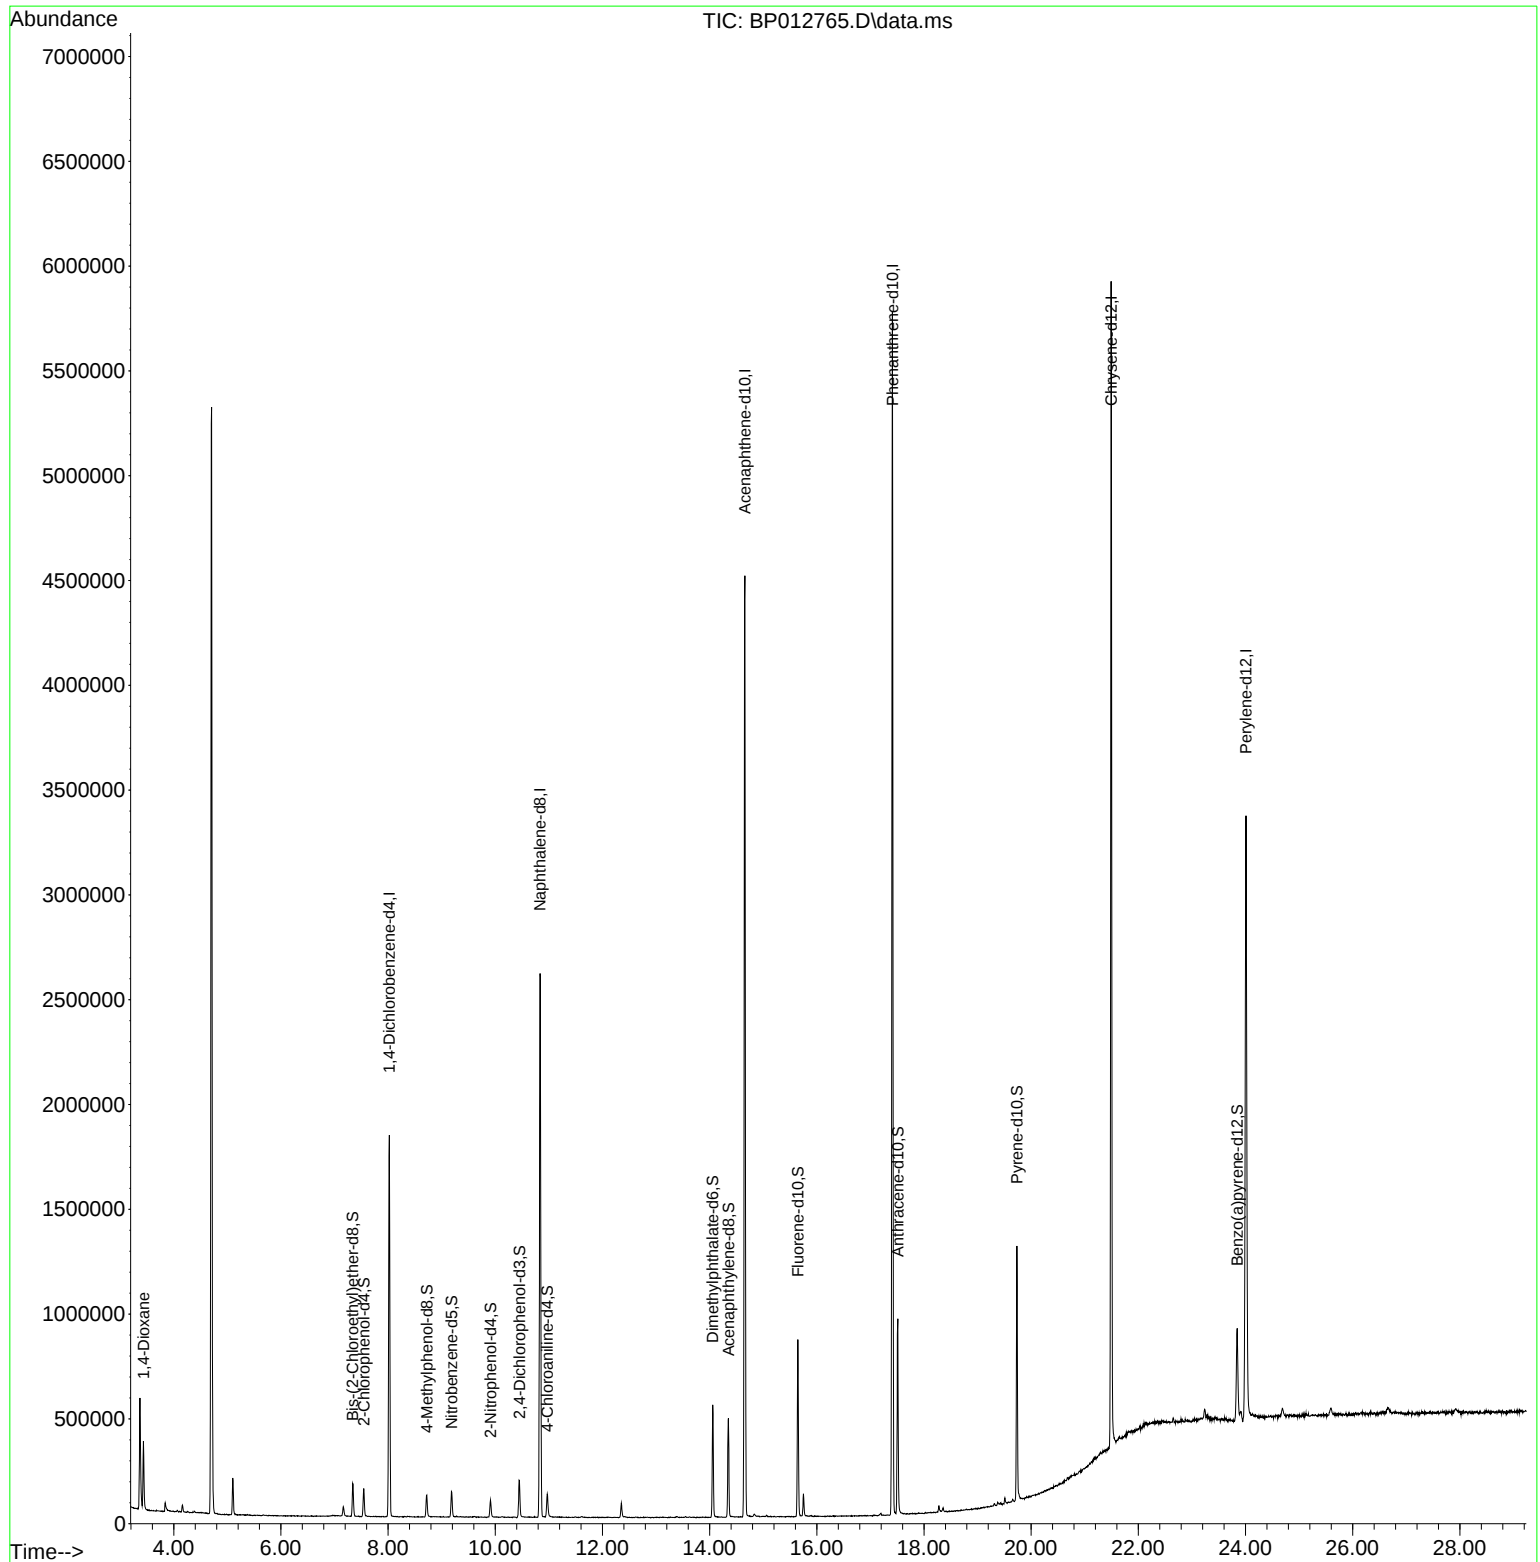

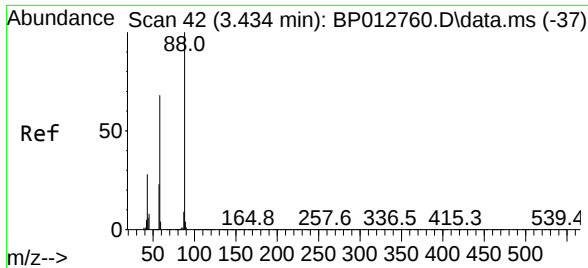

#2
 1,4-Dioxane
 Concen: 12.180 ng/uL
 RT: 3.434 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BP012765.D
 Acq: 26 Nov 2022 13:36

Instrument :
 BNA_P
 ClientSampleId :
 H0AB0DL

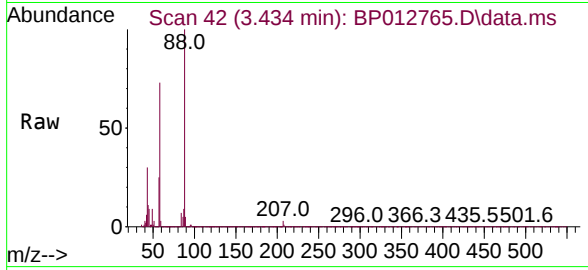

Tgt Ion: 88 Resp: 156156
 Ion Ratio Lower Upper
 88 100
 43 29.7 22.6 34.0
 58 73.4 59.6 89.4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/28/2022
 Supervised By :mohammad ahmed 11/30/2022

