

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012785.D
 Acq On : 27 Nov 2022 01:32
 Operator : CG/JU
 Sample : N5710-04
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KY3

Quant Time: Nov 27 23:02:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.017	152	533897	20.000	ng/u1	0.00
20) Naphthalene-d8	10.834	136	2417737	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.651	164	1650780	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.410	188	3670005	20.000	ng/u1	0.00
79) Chrysene-d12	21.492	240	3632852	20.000	ng/u1	0.00
88) Perylene-d12	24.010	264	3625304	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	58030	4.658	ng/uL	0.00
4) Pyridine-d5	3.823	84	261763	7.020	ng/u1	0.00
7) Phenol-d5	7.164	99	235074	5.358	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	802654	29.691	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	741350	22.176	ng/u1	0.00
15) 4-Methylphenol-d8	8.716	113	478439	13.535	ng/u1	0.00
21) Nitrobenzene-d5	9.181	128	490269	33.131	ng/u1	0.00
24) 2-Nitrophenol-d4	9.911	143	499360	31.781	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.446	165	930476	25.380	ng/u1	0.00
31) 4-Chloroaniline-d4	10.963	131	1282506	25.546	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	3780334	33.270	ng/u1	0.00
49) Acenaphthylene-d8	14.346	160	4203990	31.709	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	78186	3.860	ng/u1	0.00
60) Fluorene-d10	15.646	176	3398433	34.152	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	430919	24.567	ng/u1	0.00
73) Anthracene-d10	17.510	188	5610183	34.727	ng/u1	0.00
81) Pyrene-d10	19.734	212	6636944	31.441	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.845	264	6210922	34.879	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.434	88	82737	6.183	ng/uL	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012785.D
Acq On : 27 Nov 2022 01:32
Operator : CG/JU
Sample : N5710-04
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KY3

Quant Time: Nov 27 23:02:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration

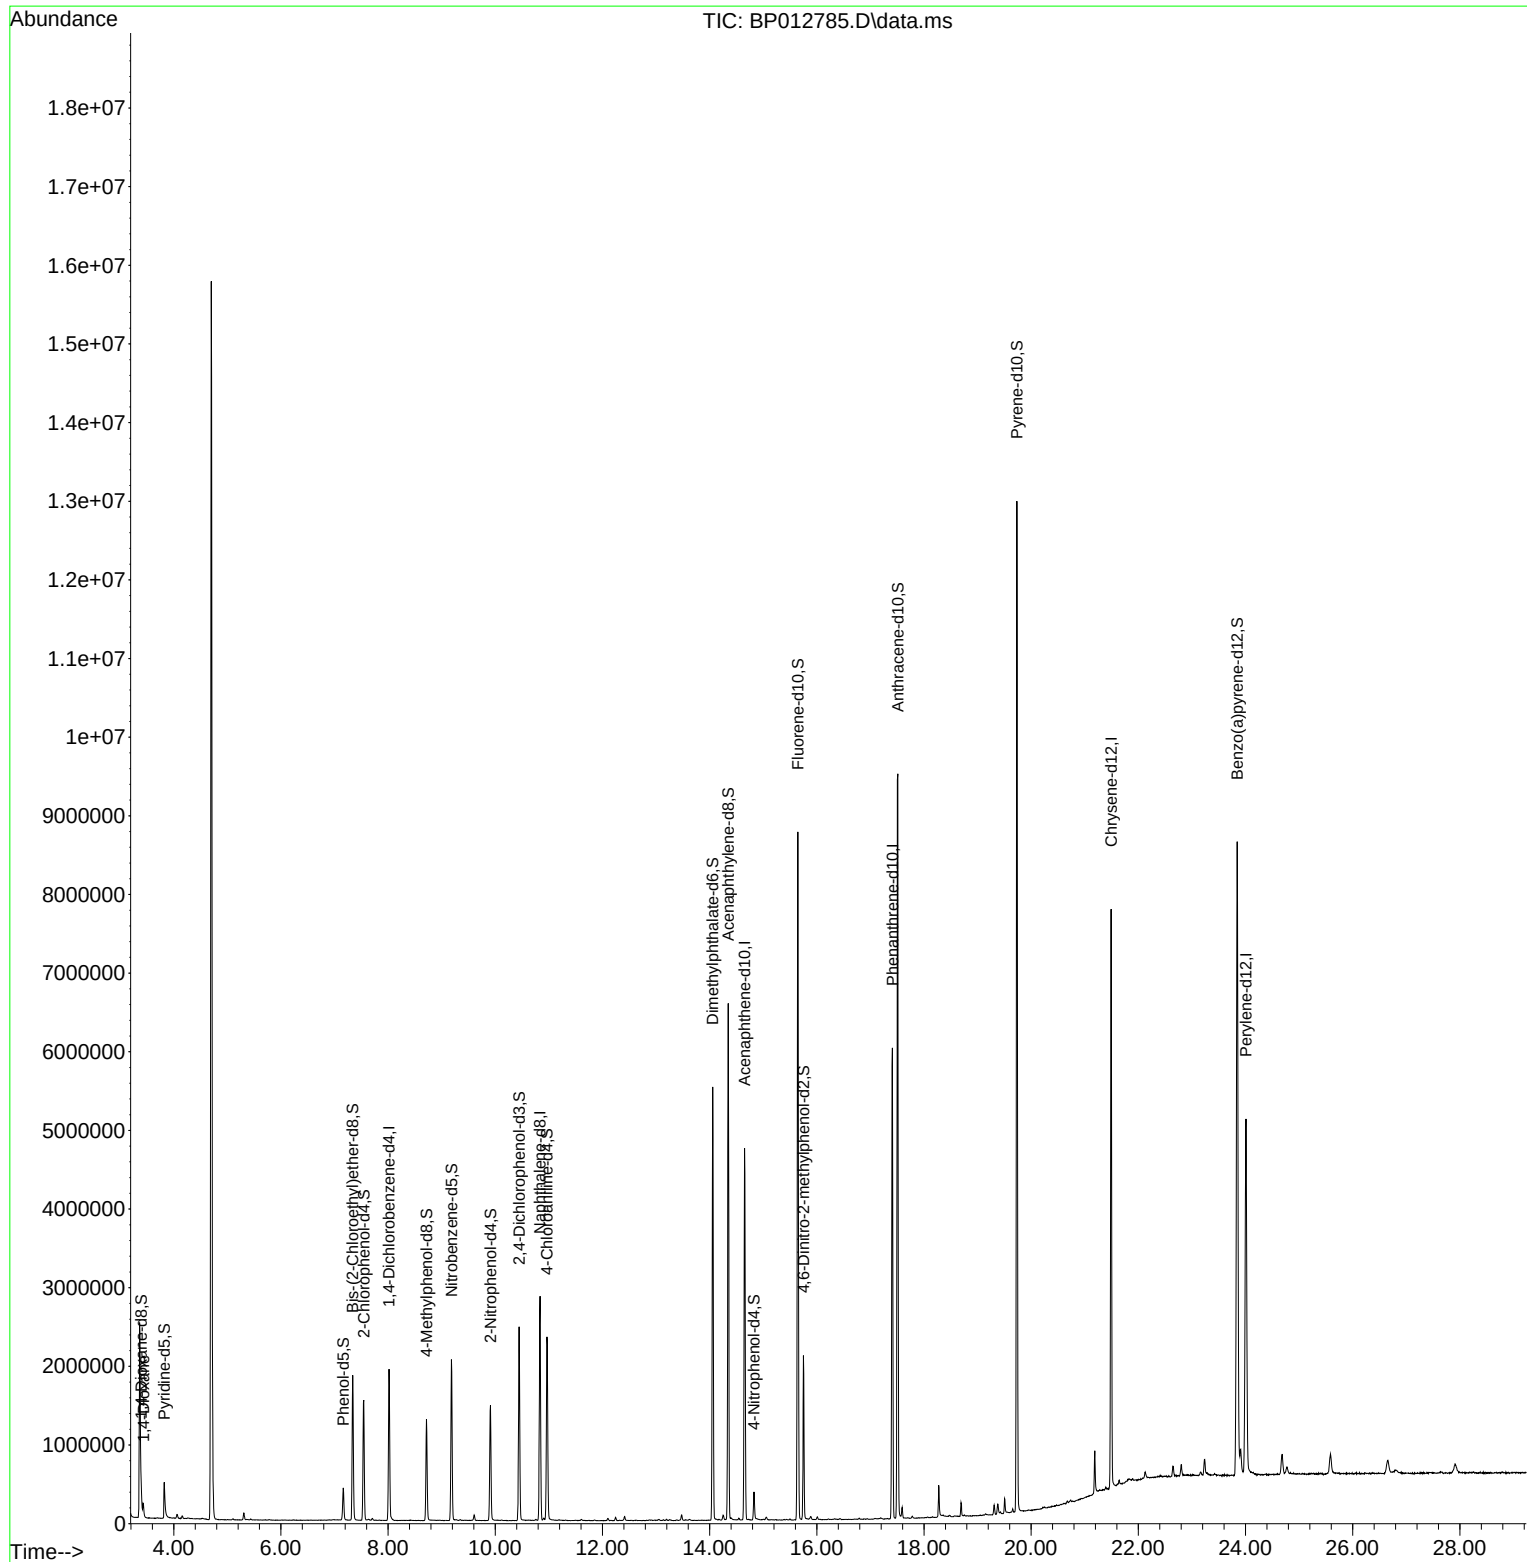

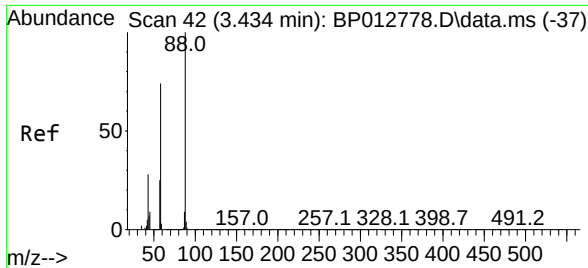

#2
 1,4-Dioxane
 Concen: 6.183 ng/uL
 RT: 3.434 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BP012785.D
 Acq: 27 Nov 2022 01:32

Instrument :
 BNA_P
 ClientSampleId :
 C0KY3

Tgt Ion: 88	Resp: 82737
Ion Ratio	Lower Upper
88	100
43	26.8 22.6 34.0
58	67.7 59.6 89.4

