

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012788.D
 Acq On : 27 Nov 2022 03:15
 Operator : CG/JU
 Sample : N5710-08
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KY7

Quant Time: Nov 27 23:02:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	542850	20.000	ng/u1	0.00
20) Naphthalene-d8	10.834	136	2479917	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.651	164	1730704	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.410	188	3768421	20.000	ng/u1	0.00
79) Chrysene-d12	21.492	240	3667681	20.000	ng/u1	0.00
88) Perylene-d12	24.009	264	3577167	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	59242	4.676	ng/uL	0.00
4) Pyridine-d5	3.822	84	255274	6.734	ng/u1	0.00
7) Phenol-d5	7.163	99	346463	7.767	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	818645	29.783	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	838664	24.674	ng/u1	0.00
15) 4-Methylphenol-d8	8.716	113	594389	16.538	ng/u1	0.00
21) Nitrobenzene-d5	9.181	128	499839	32.931	ng/u1	0.00
24) 2-Nitrophenol-d4	9.910	143	531622	32.986	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.446	165	1005868	26.748	ng/u1	0.00
31) 4-Chloroaniline-d4	10.963	131	1129712	21.938	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	3910322	32.825	ng/u1	0.00
49) Acenaphthylene-d8	14.345	160	4220233	30.362	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	146294	6.888	ng/u1	0.00
60) Fluorene-d10	15.645	176	3496070	33.510	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	515538	28.623	ng/u1	0.00
73) Anthracene-d10	17.510	188	5939760	35.807	ng/u1	0.00
81) Pyrene-d10	19.733	212	7090588	33.272	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.845	264	6444804	36.679	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.434	88	106711	7.843	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012788.D
Acq On : 27 Nov 2022 03:15
Operator : CG/JU
Sample : N5710-08
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KY7

Quant Time: Nov 27 23:02:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration

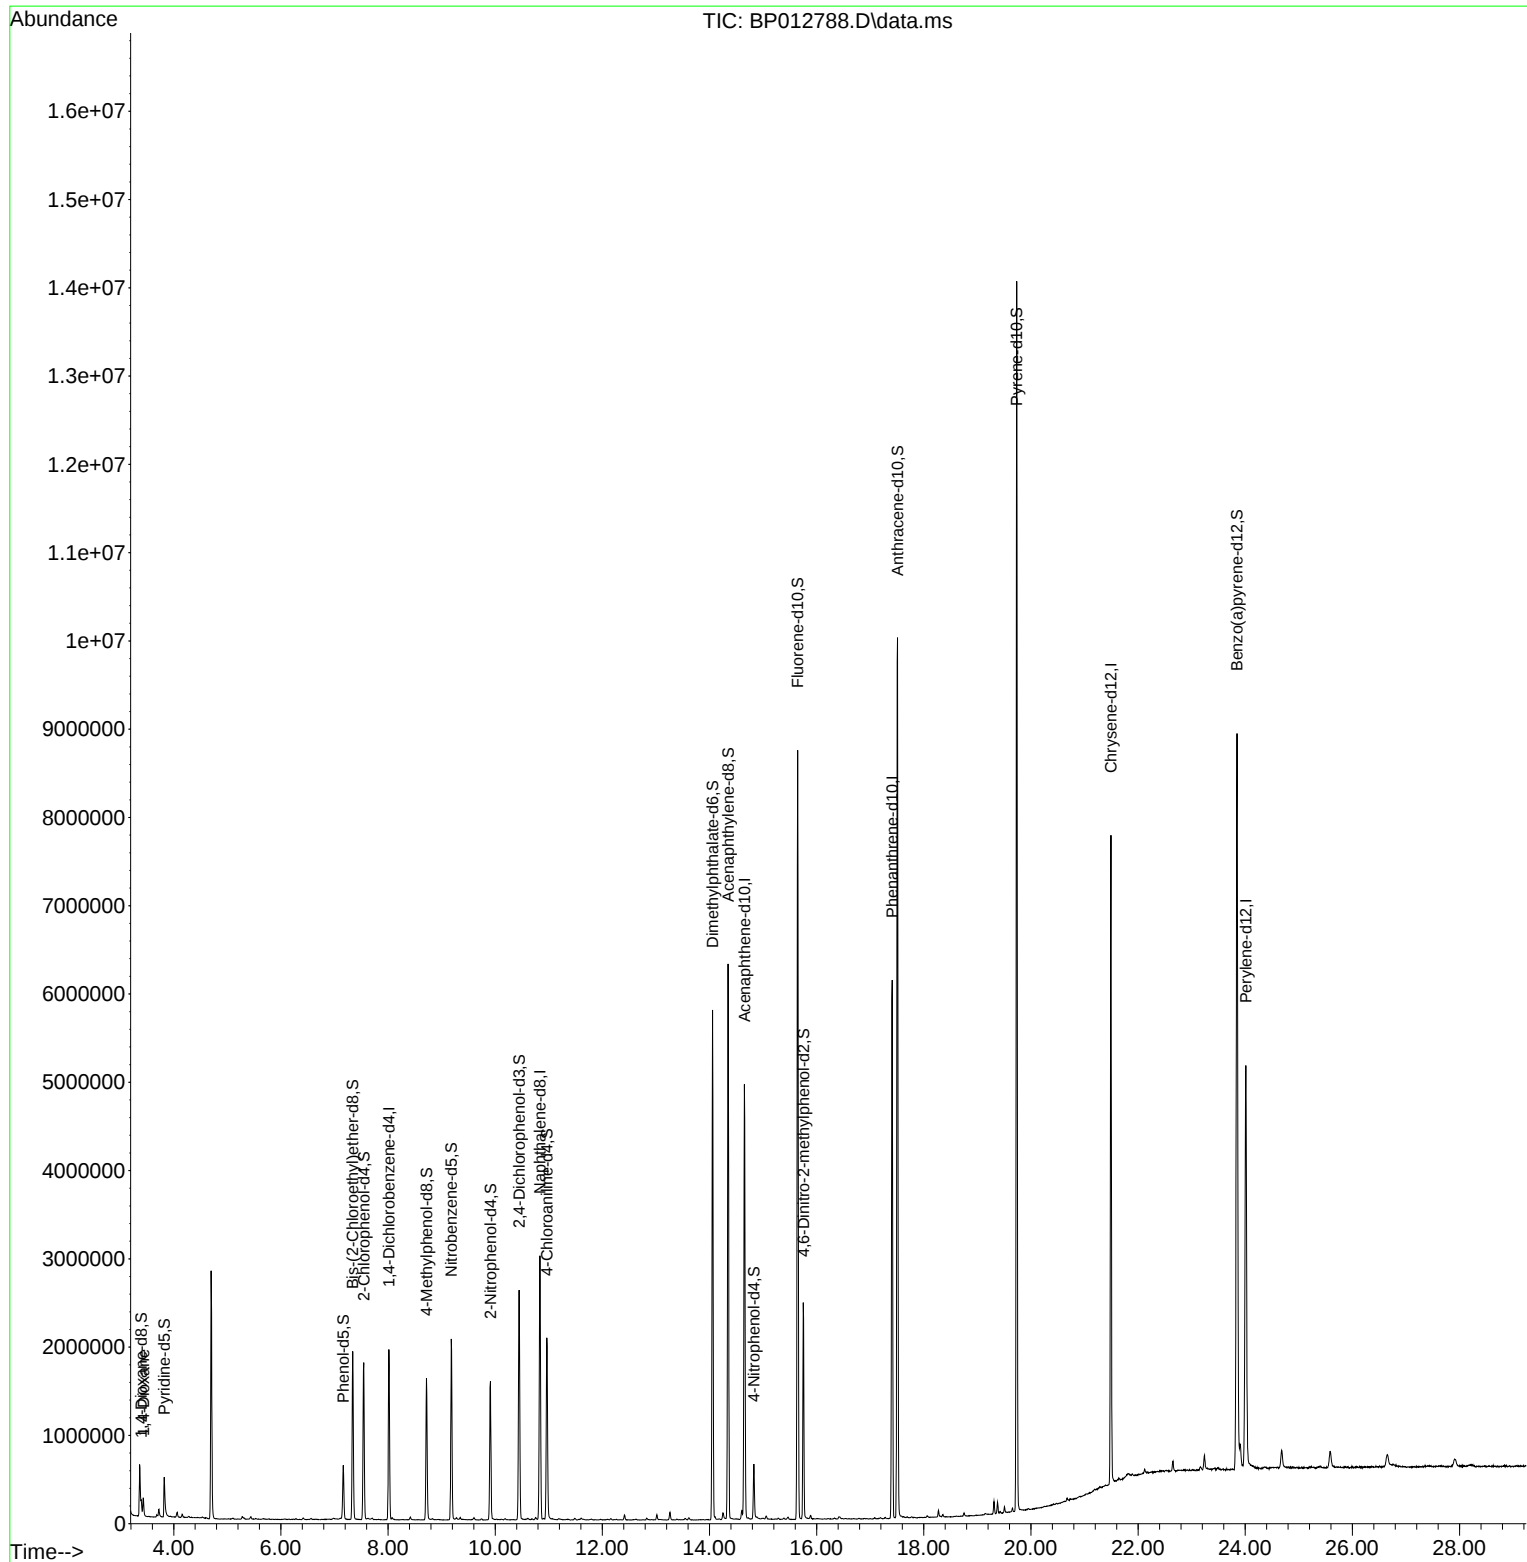

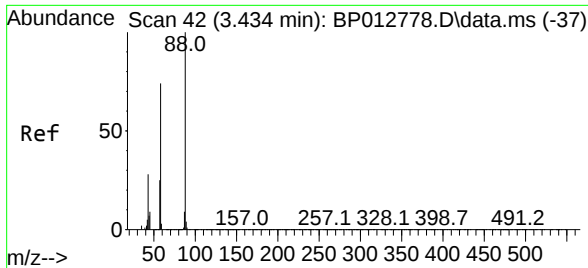

#2
 1,4-Dioxane
 Concen: 7.843 ng/uL
 RT: 3.434 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BP012788.D
 Acq: 27 Nov 2022 03:15

Instrument :
 BNA_P
 ClientSampleId :
 C0KY7

Tgt Ion: 88 Resp: 106711

Ion	Ratio	Lower	Upper
88	100		
43	29.2	22.6	34.0
58	71.2	59.6	89.4

