

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012729.D
 Acq On : 25 Nov 2022 16:34
 Operator : CG/JU
 Sample : PB149032BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK032

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012729.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	42	rVB	125986	167896	1.28%	0.131%
2	3.817	104	107	131	rBV	1539937	2384190	18.22%	1.866%
3	4.164	162	166	171	rVB	31140	43061	0.33%	0.034%
4	7.169	670	677	693	rBV	1842601	2853199	21.80%	2.233%
5	7.346	701	707	715	rBV	1580822	2499669	19.10%	1.956%
6	7.552	732	742	750	rBV	1865424	2913596	22.26%	2.280%
7	8.028	815	823	831	rBV	1568289	2495069	19.06%	1.953%
8	8.722	933	941	949	rBV	2346371	3713618	28.37%	2.906%
9	9.193	1013	1021	1034	rBV	1731856	2760909	21.09%	2.161%
10	9.916	1134	1144	1154	rBV	1388355	2230691	17.04%	1.746%
11	10.451	1228	1235	1249	rBV	2372237	3874469	29.60%	3.032%
12	10.846	1294	1302	1312	rBV	2234434	3868969	29.56%	3.028%
13	10.975	1315	1324	1338	rBV	2375443	4033230	30.82%	3.156%
14	12.422	1563	1570	1580	rBV3	40398	71447	0.55%	0.056%
15	13.557	1757	1763	1768	rVB3	8692	13194	0.10%	0.010%
16	13.634	1773	1776	1783	rVB4	8835	13949	0.11%	0.011%
17	14.069	1841	1850	1863	rBV	4740469	6573206	50.22%	5.144%
18	14.357	1892	1899	1910	rBV	5315507	7780796	59.45%	6.089%
19	14.663	1941	1951	1959	rBV	3934992	5738257	43.84%	4.490%
20	14.834	1972	1980	2004	rBV	2072154	2909388	22.23%	2.277%
21	15.069	2017	2020	2029	rVB9	10152	17551	0.13%	0.014%
22	15.657	2113	2120	2131	rBV	6931371	9921626	75.81%	7.764%
23	15.763	2131	2138	2153	rVV	1756228	2350170	17.96%	1.839%
24	15.898	2156	2161	2167	rVB	28698	47796	0.37%	0.037%
25	17.098	2360	2365	2369	rVB7	9520	15622	0.12%	0.012%
26	17.204	2378	2383	2386	rBV2	9174	16180	0.12%	0.013%
27	17.422	2412	2420	2429	rBV	4788557	6933221	52.97%	5.426%
28	17.522	2429	2437	2460	rVB	7605585	11203198	85.60%	8.767%
29	18.292	2563	2568	2574	rBV3	72717	118046	0.90%	0.092%
30	18.369	2577	2581	2586	rVV2	19750	30988	0.24%	0.024%
31	19.322	2739	2743	2748	rBV3	94160	124708	0.95%	0.098%
32	19.386	2750	2754	2758	rBV	81437	126379	0.97%	0.099%
33	19.522	2773	2777	2784	rBV3	67241	98828	0.76%	0.077%
34	19.745	2809	2815	2825	rBV	10016908	13088146	100.00%	10.242%
35	19.969	2850	2853	2858	rVB	39601	46115	0.35%	0.036%
36	21.504	3108	3114	3119	rBV	5685278	7671736	58.62%	6.004%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012729.D
Acq On : 25 Nov 2022 16:34
Operator : CG/JU
Sample : PB149032BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK032

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION

37	23.863	3507	3515	3525	rBV2	5813698	11976566	91.51%	9.372%
38	24.027	3535	3543	3559	rVB2	3323305	7060979	53.95%	5.526%




Sum of corrected areas: 127786658

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012729.D
Acq On : 25 Nov 2022 16:34
Operator : CG/JU
Sample : PB149032BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK032

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

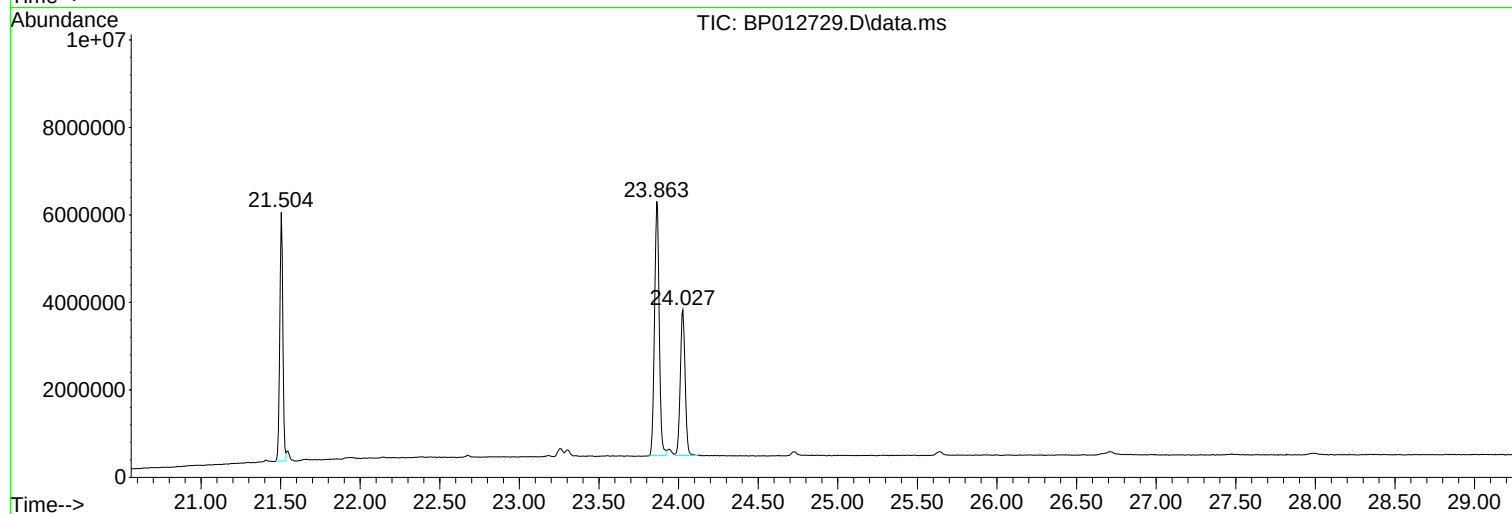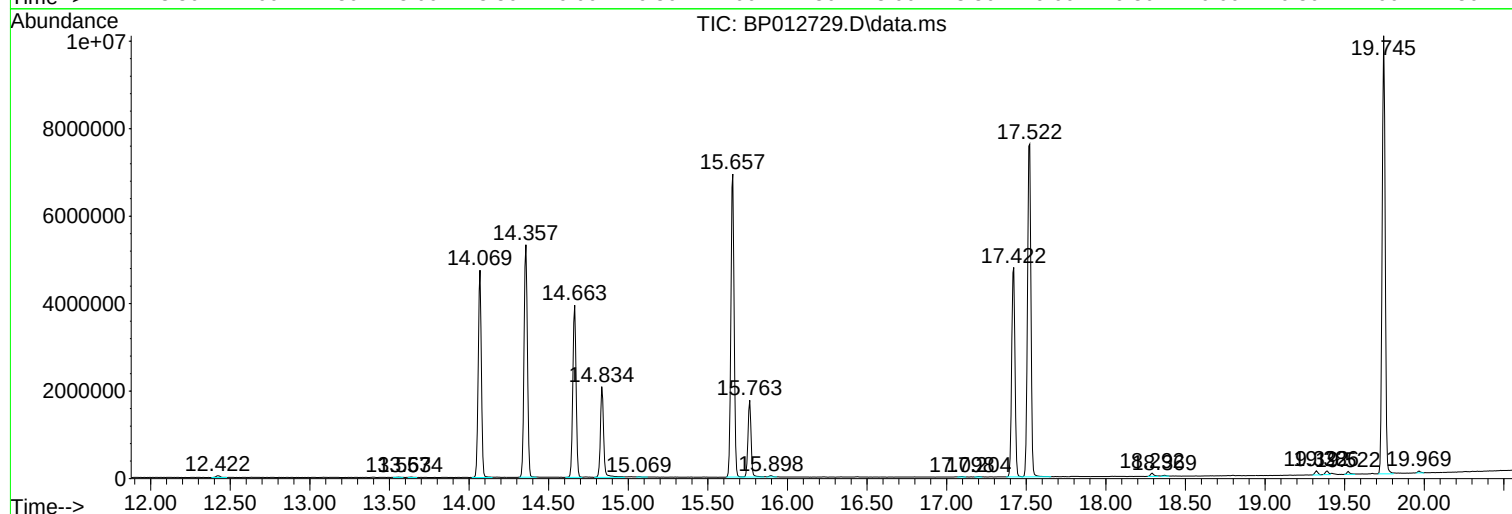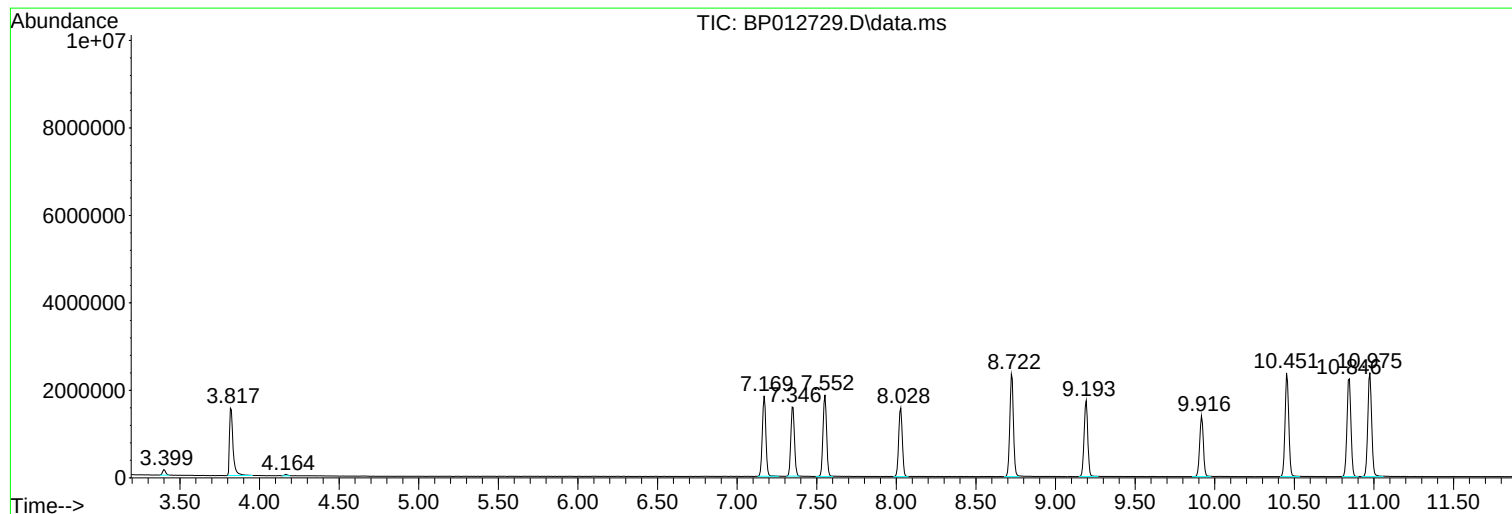

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012729.D
Acq On : 25 Nov 2022 16:34
Operator : CG/JU
Sample : PB149032BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK032

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012729.D
Acq On : 25 Nov 2022 16:34
Operator : CG/JU
Sample : PB149032BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK032

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc