

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012731.D
 Acq On : 25 Nov 2022 17:42
 Operator : CG/JU
 Sample : PB149034BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK034

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012731.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	44	rVB	137797	178717	1.28%	0.132%
2	3.817	104	107	132	rBV	1702498	2612825	18.68%	1.932%
3	4.164	162	166	172	rVB	32487	50404	0.36%	0.037%
4	7.169	670	677	687	rBV	2003457	3109073	22.22%	2.299%
5	7.346	699	707	717	rBV	1792838	2751230	19.67%	2.034%
6	7.552	733	742	751	rBV	1971637	3170710	22.66%	2.344%
7	8.022	815	822	832	rBV	1718382	2702361	19.32%	1.998%
8	8.722	933	941	956	rBV	2597614	4100674	29.31%	3.032%
9	9.187	1011	1020	1029	rBV	1885028	3027835	21.64%	2.239%
10	9.916	1136	1144	1153	rBV	1556861	2443789	17.47%	1.807%
11	10.452	1226	1235	1250	rBV	2662642	4295618	30.70%	3.176%
12	10.840	1292	1301	1310	rBV	2545784	4258875	30.44%	3.149%
13	10.969	1314	1323	1339	rBV	2568908	4470404	31.95%	3.305%
14	12.422	1563	1570	1575	rBV2	44211	72764	0.52%	0.054%
15	13.557	1756	1763	1771	rBV2	20950	34397	0.25%	0.025%
16	13.640	1771	1777	1784	rVB3	10219	21020	0.15%	0.016%
17	14.063	1842	1849	1865	rBV	5034974	7141709	51.05%	5.280%
18	14.351	1891	1898	1908	rBV	5745186	8549460	61.11%	6.321%
19	14.657	1942	1950	1959	rBV	4219617	6223228	44.48%	4.601%
20	14.834	1972	1980	2001	rBV	2190802	3118215	22.29%	2.306%
21	15.069	2015	2020	2026	rVB9	11205	18895	0.14%	0.014%
22	15.651	2112	2119	2131	rBV	7519397	10841161	77.49%	8.016%
23	15.757	2131	2137	2152	rVV	1845111	2544509	18.19%	1.881%
24	15.892	2155	2160	2167	rVB2	33312	56631	0.40%	0.042%
25	16.228	2211	2217	2221	rBV7	7977	14005	0.10%	0.010%
26	16.439	2248	2253	2256	rBV4	9381	14101	0.10%	0.010%
27	17.198	2379	2382	2389	rVB4	11639	19063	0.14%	0.014%
28	17.416	2412	2419	2429	rBV	5210908	7434061	53.14%	5.497%
29	17.516	2429	2436	2454	rVV	8554540	12086825	86.40%	8.937%
30	18.286	2563	2567	2574	rBV3	57766	96108	0.69%	0.071%
31	19.322	2738	2743	2749	rVB	95259	134108	0.96%	0.099%
32	19.386	2749	2754	2758	rBV	94711	145302	1.04%	0.107%
33	19.516	2773	2776	2784	rBV5	49945	86563	0.62%	0.064%
34	19.745	2808	2815	2826	rBV	10401307	13989983	100.00%	10.344%
35	21.504	3108	3114	3119	rBV	5762968	7650010	54.68%	5.656%
36	23.857	3507	3514	3524	rBV2	5482809	11152976	79.72%	8.246%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012731.D
Acq On : 25 Nov 2022 17:42
Operator : CG/JU
Sample : PB149034BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK034

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION

37	24.021	3535	3542	3559	rVB2	3115609	6633184	47.41%	4.904%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 135250793

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012731.D
Acq On : 25 Nov 2022 17:42
Operator : CG/JU
Sample : PB149034BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK034

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

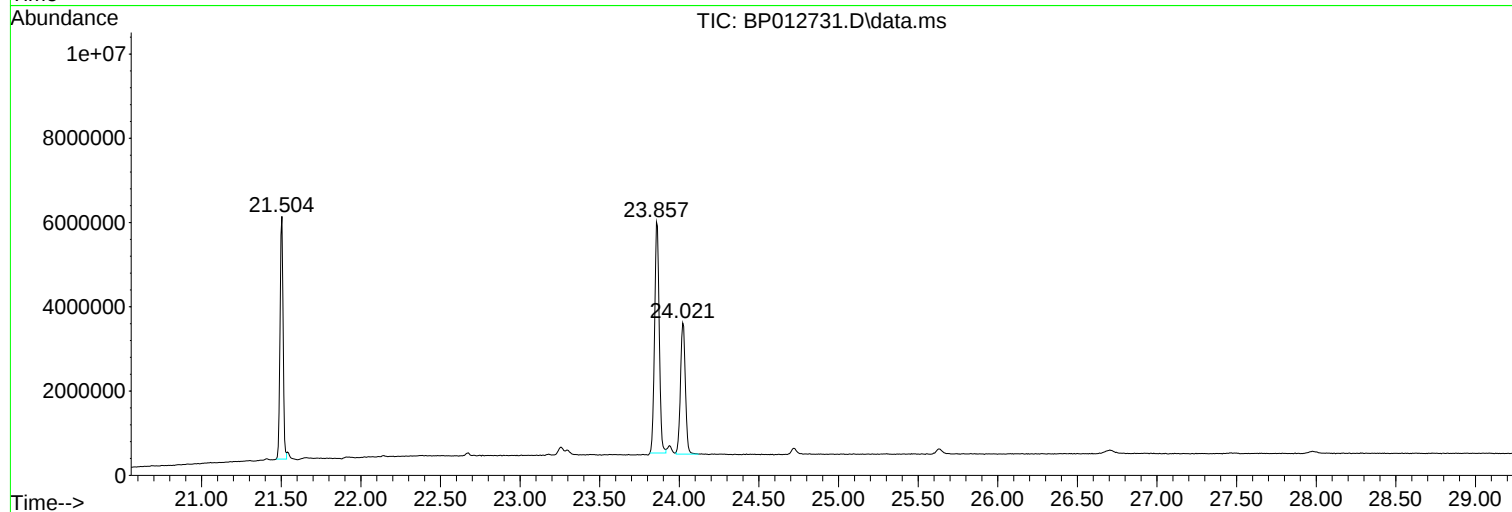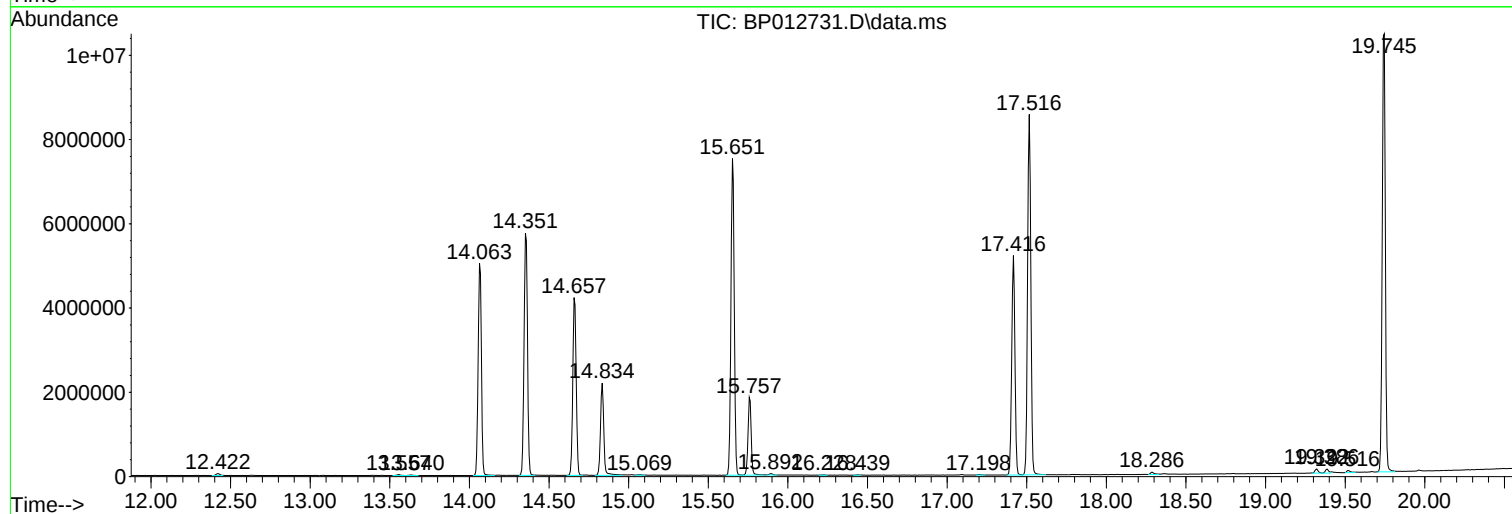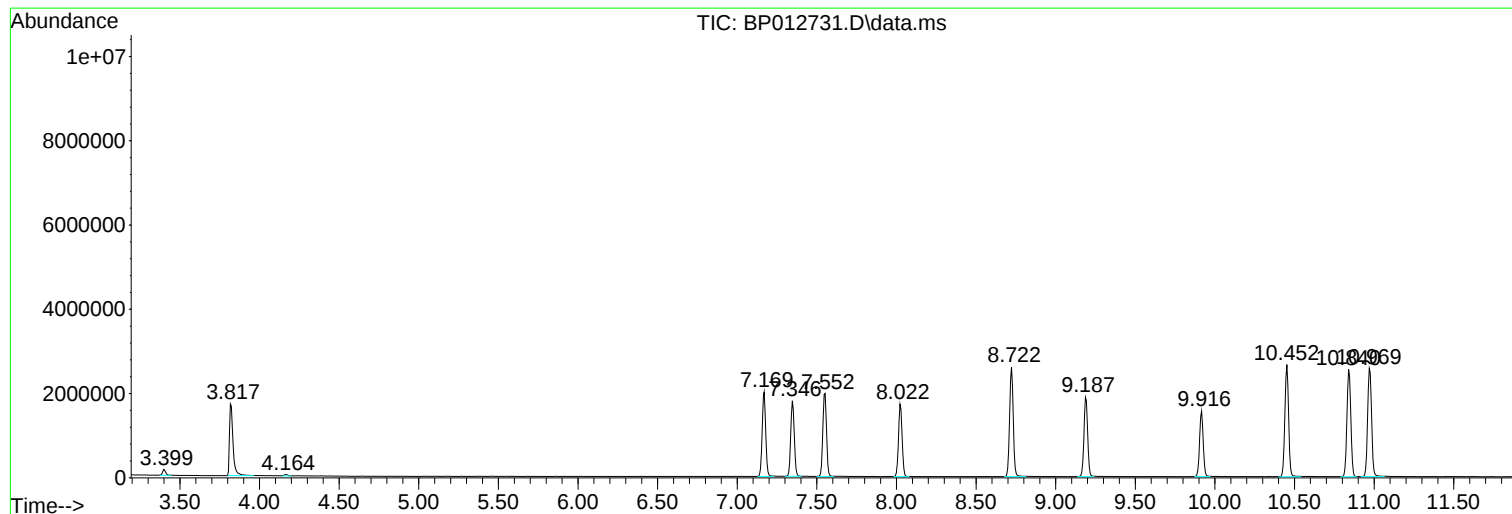

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012731.D
Acq On : 25 Nov 2022 17:42
Operator : CG/JU
Sample : PB149034BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK034

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012731.D
Acq On : 25 Nov 2022 17:42
Operator : CG/JU
Sample : PB149034BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK034

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc