

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012735.D
 Acq On : 25 Nov 2022 19:59
 Operator : CG/JU
 Sample : N5592-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012735.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	34	rBV	148395	216937	1.72%	0.186%
2	3.399	34	36	40	rVV	121079	148904	1.18%	0.127%
3	3.434	40	42	50	rVB	63392	87259	0.69%	0.075%
4	3.687	82	85	90	rBV3	10649	16933	0.13%	0.014%
5	3.822	105	108	125	rBV	634774	956915	7.59%	0.819%
6	4.064	144	149	154	rBV	47006	75628	0.60%	0.065%
7	4.164	162	166	171	rVB	36133	49238	0.39%	0.042%
8	4.705	251	258	266	rBV	696507	1010426	8.01%	0.865%
9	6.969	639	643	647	rBV4	11418	15690	0.12%	0.013%
10	7.169	670	677	687	rBV	463768	746156	5.92%	0.638%
11	7.346	699	707	717	rBV	1807230	2806549	22.26%	2.401%
12	7.546	734	741	752	rBV	1594649	2543103	20.17%	2.176%
13	7.646	755	758	763	rVB6	10610	17564	0.14%	0.015%
14	8.022	814	822	829	rBV	1784222	2774021	22.00%	2.373%
15	8.081	829	832	836	rVB3	11829	18406	0.15%	0.016%
16	8.375	878	882	889	rVB9	7919	14685	0.12%	0.013%
17	8.722	932	941	953	rBV	1422788	2231566	17.70%	1.909%
18	9.187	1011	1020	1032	rBV	1901357	3089022	24.50%	2.643%
19	9.281	1032	1036	1042	rVB3	19607	35124	0.28%	0.030%
20	9.616	1087	1093	1102	rVB4	15251	29433	0.23%	0.025%
21	9.916	1136	1144	1156	rBV	1409414	2321461	18.41%	1.986%
22	10.116	1173	1178	1185	rVB6	12317	21992	0.17%	0.019%
23	10.334	1209	1215	1219	rBV8	6824	13989	0.11%	0.012%
24	10.451	1227	1235	1245	rBV	2406764	3984716	31.61%	3.409%
25	10.840	1292	1301	1311	rBV	2558213	4329521	34.34%	3.704%
26	10.969	1314	1323	1342	rBV	2077487	3594089	28.51%	3.075%
27	11.275	1366	1375	1380	rVB9	6200	15741	0.12%	0.013%
28	11.610	1427	1432	1438	rBV3	26159	41764	0.33%	0.036%
29	12.416	1561	1569	1574	rBV	44351	75042	0.60%	0.064%
30	13.022	1668	1672	1677	rBV5	10842	16002	0.13%	0.014%
31	13.275	1711	1715	1720	rVB6	14080	19812	0.16%	0.017%
32	13.557	1756	1763	1769	rBV8	9042	19857	0.16%	0.017%
33	13.634	1769	1776	1781	rVV2	10032	15750	0.12%	0.013%
34	13.839	1807	1811	1816	rBV2	14319	19393	0.15%	0.017%
35	14.063	1842	1849	1861	rBV	5138400	7017687	55.66%	6.004%
36	14.351	1891	1898	1907	rBV	5678954	8534615	67.70%	7.302%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012735.D
 Acq On : 25 Nov 2022 19:59
 Operator : CG/JU
 Sample : N5592-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	14.657	1943	1950	1959	rBV	4205383	6166120	48.91%	5.276%
38	14.828	1972	1979	1998	rBV	297944	529031	4.20%	0.453%
39	15.069	2015	2020	2025	rVB5	32019	54729	0.43%	0.047%
40	15.463	2083	2087	2092	rBV3	13289	27059	0.21%	0.023%
41	15.651	2112	2119	2131	rBV	7734400	10937481	86.76%	9.358%
42	15.757	2131	2137	2152	rVV	1733878	2292757	18.19%	1.962%
43	15.892	2154	2160	2167	rVB	36372	64847	0.51%	0.055%
44	16.439	2249	2253	2259	rVB7	11229	18024	0.14%	0.015%
45	16.798	2311	2314	2320	rVB7	14115	22402	0.18%	0.019%
46	17.092	2360	2364	2368	rVB5	9124	14007	0.11%	0.012%
47	17.416	2412	2419	2428	rBV	5094989	6977337	55.34%	5.970%
48	17.516	2429	2436	2455	rVB	8499770	12002258	95.20%	10.269%
49	17.698	2464	2467	2474	rVB3	9960	15440	0.12%	0.013%
50	18.080	2528	2532	2536	rVB4	22993	31298	0.25%	0.027%
51	18.286	2560	2567	2574	rBV	229192	315319	2.50%	0.270%
52	18.363	2576	2580	2590	rVB	55431	94045	0.75%	0.080%
53	19.322	2738	2743	2747	rBV	88511	133435	1.06%	0.114%
54	19.386	2749	2754	2760	rBV	93937	179776	1.43%	0.154%
55	19.516	2772	2776	2785	rBV	139259	185423	1.47%	0.159%
56	19.669	2799	2802	2805	rVB3	24337	24918	0.20%	0.021%
57	19.739	2808	2814	2827	rBV	9390940	12607174	100.00%	10.787%
58	21.198	3059	3062	3068	rBV3	105865	131503	1.04%	0.113%
59	21.498	3108	3113	3119	rBV	3905143	5309328	42.11%	4.543%
60	23.857	3507	3514	3523	rBV2	3767247	7560102	59.97%	6.468%
61	24.021	3535	3542	3556	rVB2	2057041	4259380	33.79%	3.644%




Sum of corrected areas: 116878183

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012735.D
Acq On : 25 Nov 2022 19:59
Operator : CG/JU
Sample : N5592-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

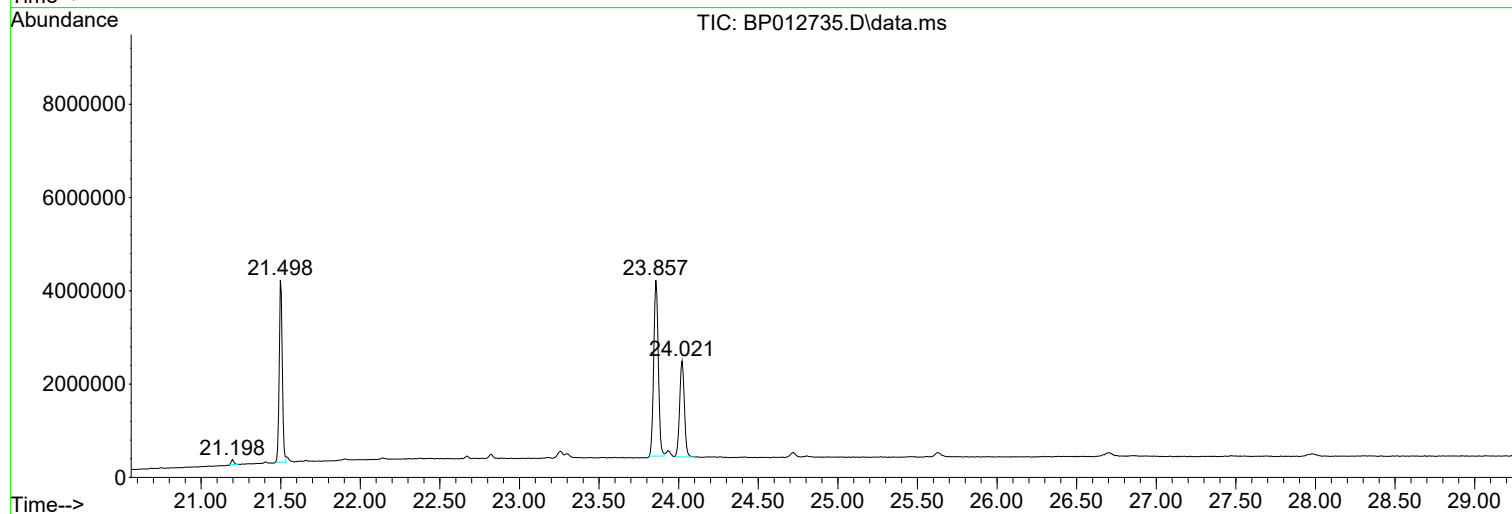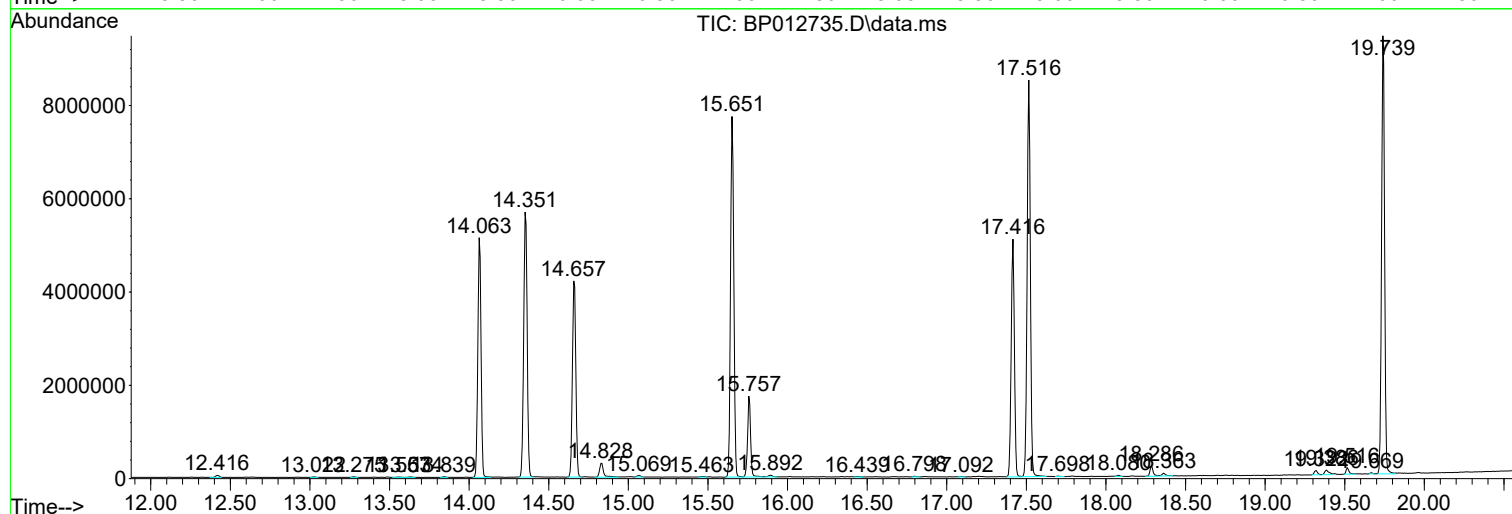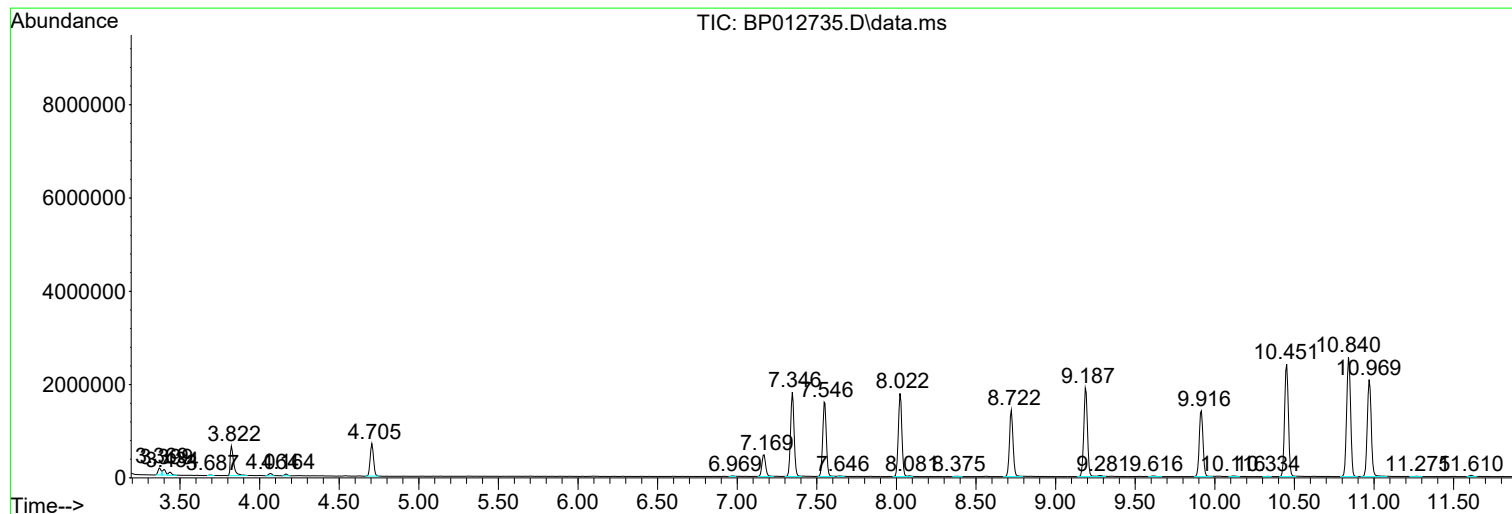

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012735.D
Acq On : 25 Nov 2022 19:59
Operator : CG/JU
Sample : N5592-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012735.D
Acq On : 25 Nov 2022 19:59
Operator : CG/JU
Sample : N5592-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc