

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012738.D
 Acq On : 25 Nov 2022 21:41
 Operator : CG/JU
 Sample : N5592-15
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012738.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	33	rBV2	65914	87417	0.57%	0.066%
2	3.399	33	36	40	rVV	116307	162313	1.05%	0.122%
3	3.434	40	42	49	rVB	81349	108906	0.71%	0.082%
4	3.822	105	108	123	rBV	634974	941724	6.10%	0.710%
5	4.069	145	150	155	rVB	55738	85830	0.56%	0.065%
6	4.163	162	166	171	rBV	35793	49581	0.32%	0.037%
7	4.540	227	230	237	rVB7	11111	15760	0.10%	0.012%
8	4.705	252	258	269	rVB	693497	1018547	6.60%	0.767%
9	6.975	638	644	648	rBV4	12705	21482	0.14%	0.016%
10	7.163	670	676	687	rBV	523777	844829	5.48%	0.637%
11	7.346	699	707	716	rBV	2041407	3141370	20.36%	2.367%
12	7.546	733	741	752	rBV	1821624	2882590	18.68%	2.172%
13	7.646	754	758	762	rVB6	11197	17132	0.11%	0.013%
14	8.022	814	822	830	rBV	1850099	2854424	18.50%	2.151%
15	8.722	933	941	953	rBV	1572131	2526890	16.38%	1.904%
16	9.187	1011	1020	1031	rBV	2150126	3434011	22.26%	2.587%
17	9.293	1031	1038	1044	rVV	110587	200510	1.30%	0.151%
18	9.340	1044	1046	1055	rVB10	8216	20240	0.13%	0.015%
19	9.616	1087	1093	1098	rVB3	12574	23684	0.15%	0.018%
20	9.916	1135	1144	1158	rBV	1619226	2671446	17.31%	2.013%
21	10.116	1175	1178	1186	rVB6	9132	15486	0.10%	0.012%
22	10.451	1226	1235	1250	rBV	2788219	4572409	29.64%	3.445%
23	10.840	1292	1301	1311	rBV	2689544	4495871	29.14%	3.387%
24	10.969	1315	1323	1337	rBV	2490855	4213844	27.31%	3.175%
25	11.610	1427	1432	1437	rBV5	14927	26401	0.17%	0.020%
26	12.416	1564	1569	1574	rBV2	45151	74772	0.48%	0.056%
27	13.022	1668	1672	1677	rBV4	12266	16318	0.11%	0.012%
28	13.269	1708	1714	1720	rVB4	13935	22330	0.14%	0.017%
29	13.634	1771	1776	1781	rVB5	10361	18057	0.12%	0.014%
30	13.839	1805	1811	1816	rBV	15746	22994	0.15%	0.017%
31	14.063	1842	1849	1862	rBV	5635724	8082773	52.39%	6.090%
32	14.351	1891	1898	1912	rBV	6776288	9537127	61.81%	7.186%
33	14.657	1943	1950	1958	rBV	4510162	6417619	41.59%	4.835%
34	14.734	1960	1963	1968	rVB7	11063	16064	0.10%	0.012%
35	14.828	1973	1979	1988	rBV	395968	602375	3.90%	0.454%
36	15.016	2005	2011	2015	rBV7	9220	17099	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012738.D
 Acq On : 25 Nov 2022 21:41
 Operator : CG/JU
 Sample : N5592-15
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	15.063	2015	2019	2027	rVB4	43037	68875	0.45%	0.052%
38	15.463	2083	2087	2092	rBV3	12931	23995	0.16%	0.018%
39	15.651	2112	2119	2130	rBV	8735360	12382344	80.25%	9.329%
40	15.757	2130	2137	2155	rVV	2156944	2853627	18.50%	2.150%
41	15.892	2155	2160	2167	rVB2	37185	61799	0.40%	0.047%
42	16.222	2210	2216	2220	rBV8	12758	19271	0.12%	0.015%
43	16.433	2249	2252	2257	rVB6	12077	15445	0.10%	0.012%
44	16.798	2310	2314	2318	rBV5	13324	19514	0.13%	0.015%
45	17.416	2412	2419	2428	rBV	5205042	7419650	48.09%	5.590%
46	17.516	2429	2436	2455	rVB	9681122	14054628	91.09%	10.589%
47	17.786	2478	2482	2489	rVB5	8627	16701	0.11%	0.013%
48	17.916	2498	2504	2506	rBV7	10686	19689	0.13%	0.015%
49	18.075	2528	2531	2535	rVB2	18321	20084	0.13%	0.015%
50	18.286	2561	2567	2575	rBV	267138	396656	2.57%	0.299%
51	18.363	2577	2580	2587	rVB	35177	52708	0.34%	0.040%
52	18.580	2614	2617	2621	rBV6	10859	16312	0.11%	0.012%
53	19.316	2737	2742	2748	rBV	119842	182215	1.18%	0.137%
54	19.380	2749	2753	2760	rBV	116214	199050	1.29%	0.150%
55	19.516	2772	2776	2787	rBV	214482	281696	1.83%	0.212%
56	19.669	2799	2802	2806	rVB4	22758	23979	0.16%	0.018%
57	19.739	2808	2814	2828	rBV	11654552	15429058	100.00%	11.625%
58	21.198	3059	3062	3065	rBV2	78463	95273	0.62%	0.072%
59	21.498	3108	3113	3119	rBV	4507796	6018422	39.01%	4.534%
60	23.857	3506	3514	3523	rBV2	4506947	9267858	60.07%	6.983%
61	24.015	3534	3541	3555	rVB2	2128775	4528306	29.35%	3.412%




Sum of corrected areas: 132727380

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012738.D
Acq On : 25 Nov 2022 21:41
Operator : CG/JU
Sample : N5592-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

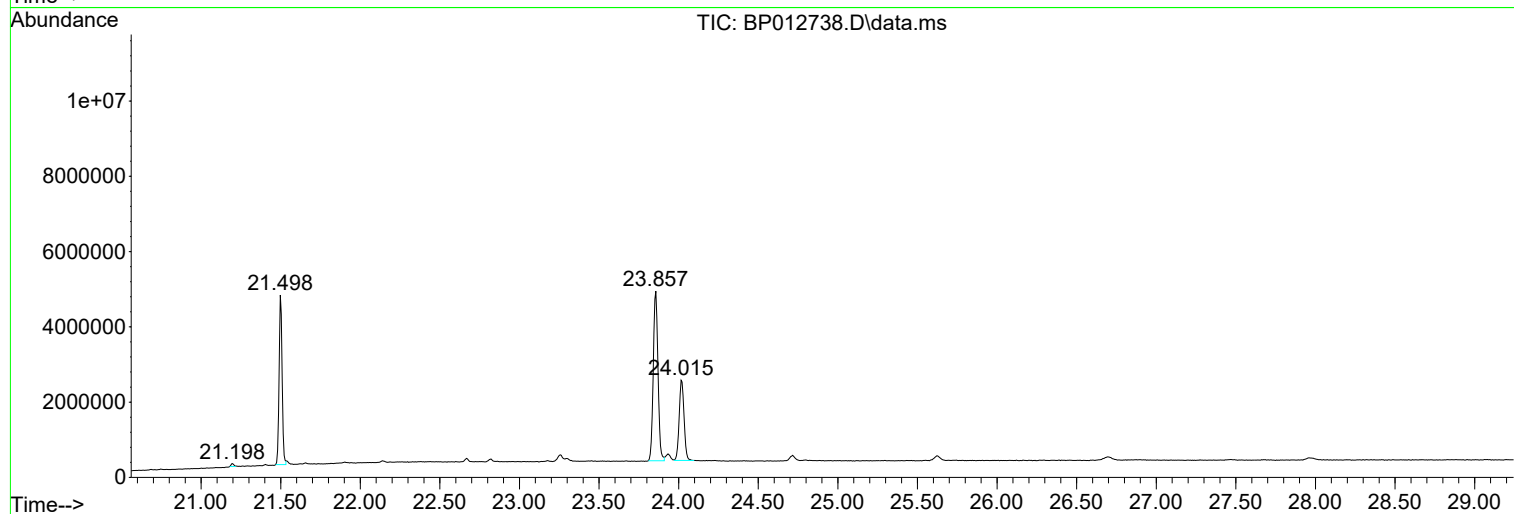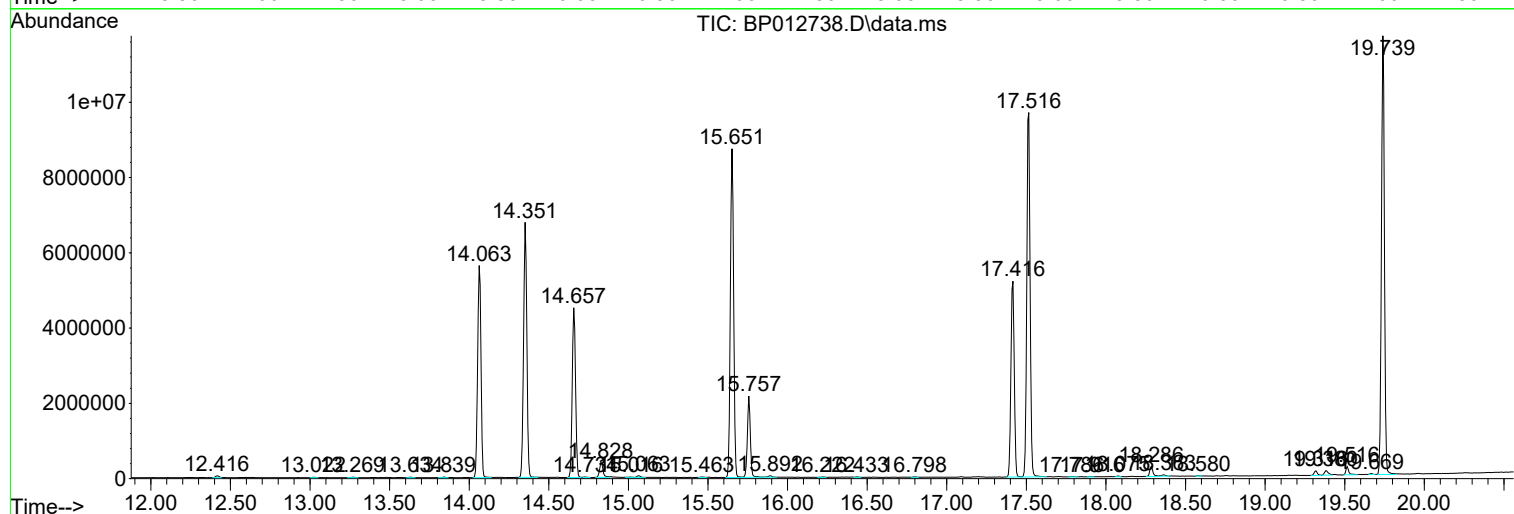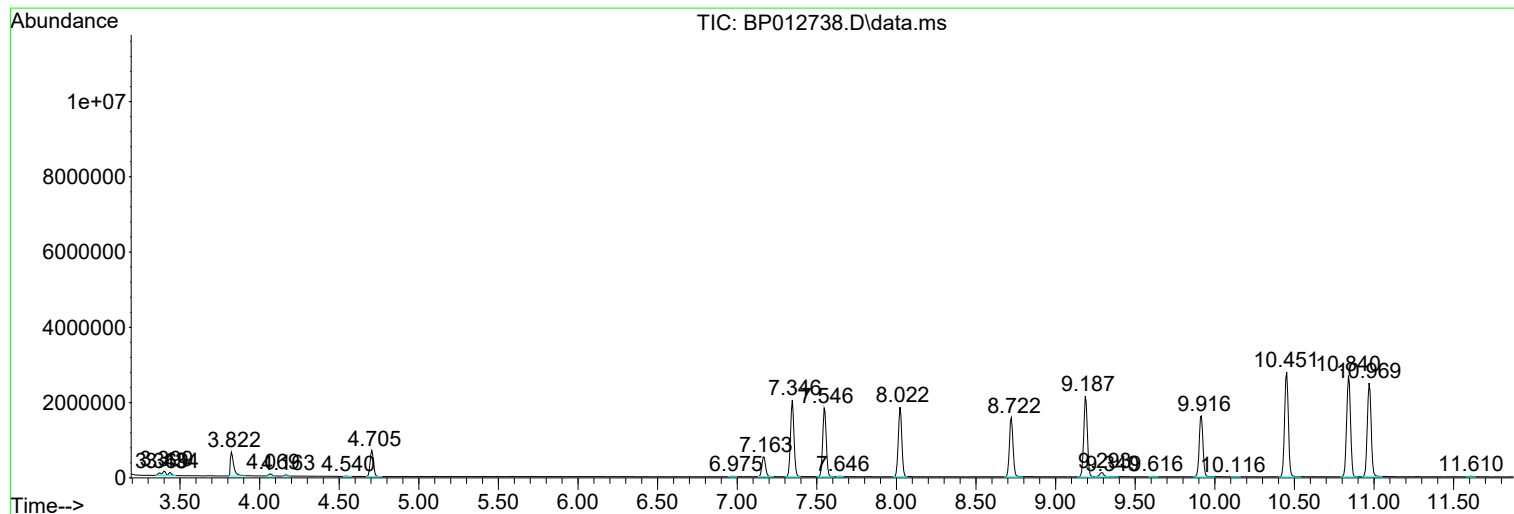

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012738.D
Acq On : 25 Nov 2022 21:41
Operator : CG/JU
Sample : N5592-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012738.D
Acq On : 25 Nov 2022 21:41
Operator : CG/JU
Sample : N5592-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc