

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012740.D
 Acq On : 25 Nov 2022 22:49
 Operator : CG/JU
 Sample : N5592-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012740.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	26	31	33	rBV	86811	118877	0.64%	0.074%
2	3.399	33	36	39	rVV	125463	162876	0.88%	0.102%
3	3.434	39	42	48	rVB	94900	129826	0.70%	0.081%
4	3.687	81	85	94	rVB3	14377	28986	0.16%	0.018%
5	3.823	105	108	125	rBV	560591	842621	4.53%	0.528%
6	4.064	145	149	156	rVB	47442	78453	0.42%	0.049%
7	4.164	161	166	171	rBV	39014	55546	0.30%	0.035%
8	4.705	252	258	270	rVB	808658	1213528	6.53%	0.760%
9	7.164	668	676	689	rBV	484889	780159	4.20%	0.489%
10	7.346	697	707	715	rBV	1923735	2988975	16.08%	1.873%
11	7.546	733	741	753	rBV	1672859	2630581	14.15%	1.648%
12	7.640	753	757	763	rVB7	11467	20501	0.11%	0.013%
13	8.022	815	822	829	rBV	2120220	3317152	17.84%	2.078%
14	8.081	829	832	839	rVB4	15055	24887	0.13%	0.016%
15	8.722	933	941	954	rBV	1420389	2297222	12.36%	1.439%
16	9.187	1011	1020	1032	rBV	2061607	3288624	17.69%	2.060%
17	9.281	1032	1036	1041	rVB3	17546	31268	0.17%	0.020%
18	9.616	1089	1093	1100	rVB2	21036	33880	0.18%	0.021%
19	9.910	1133	1143	1154	rBV	1458618	2404331	12.93%	1.506%
20	10.452	1227	1235	1249	rBV	2557192	4201460	22.60%	2.632%
21	10.840	1293	1301	1311	rBV	3238643	5331295	28.68%	3.340%
22	10.969	1314	1323	1340	rBV	2374301	4016024	21.60%	2.516%
23	12.416	1562	1569	1579	rVB	49008	80049	0.43%	0.050%
24	13.269	1709	1714	1721	rBV6	13126	23139	0.12%	0.014%
25	13.628	1771	1775	1781	rVB2	11400	19776	0.11%	0.012%
26	14.063	1842	1849	1860	rBV	6126006	8532353	45.90%	5.346%
27	14.351	1891	1898	1908	rBV	6507462	9605721	51.67%	6.018%
28	14.557	1929	1933	1937	rVB3	14733	21082	0.11%	0.013%
29	14.657	1942	1950	1959	rBV	5363629	8021232	43.15%	5.026%
30	14.828	1973	1979	1986	rBV	443851	672727	3.62%	0.421%
31	15.063	2014	2019	2025	rVB4	47480	74369	0.40%	0.047%
32	15.469	2082	2088	2092	rBV4	11221	23152	0.12%	0.015%
33	15.651	2112	2119	2131	rBV	9544777	13324242	71.68%	8.348%
34	15.757	2131	2137	2149	rVV	2411235	3089953	16.62%	1.936%
35	15.892	2155	2160	2170	rVB	41163	73682	0.40%	0.046%
36	16.340	2232	2236	2239	rBV4	12258	19089	0.10%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012740.D
 Acq On : 25 Nov 2022 22:49
 Operator : CG/JU
 Sample : N5592-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	16.434	2250	2252	2257	rVB5	12869	18820	0.10%	0.012%
38	16.798	2310	2314	2319	rBV5	19506	27337	0.15%	0.017%
39	17.092	2360	2364	2369	rVB6	14489	23944	0.13%	0.015%
40	17.198	2379	2382	2392	rVB4	16574	37721	0.20%	0.024%
41	17.416	2412	2419	2428	rBV	6671819	9808676	52.77%	6.146%
42	17.516	2429	2436	2453	rVV	10495893	15653524	84.21%	9.808%
43	17.792	2478	2483	2487	rBV5	48931	74538	0.40%	0.047%
44	18.081	2528	2532	2537	rVB	60240	72759	0.39%	0.046%
45	18.286	2562	2567	2575	rBV	467823	677150	3.64%	0.424%
46	19.316	2738	2742	2748	rBV2	180834	315174	1.70%	0.197%
47	19.381	2749	2753	2759	rVV	169616	301579	1.62%	0.189%
48	19.516	2772	2776	2780	rBV	347012	429354	2.31%	0.269%
49	19.739	2808	2814	2820	rBV	14136413	18588898	100.00%	11.647%
50	21.192	3058	3061	3072	rBV	295583	418785	2.25%	0.262%
51	21.498	3107	3113	3127	rBV	7767656	10573130	56.88%	6.625%
52	22.816	3333	3337	3344	rVB	321077	472738	2.54%	0.296%
53	23.857	3506	3514	3523	rBV2	7617891	15420130	82.95%	9.662%
54	24.021	3534	3542	3556	rVB2	4261446	9111879	49.02%	5.709%




Sum of corrected areas: 159603774

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012740.D
Acq On : 25 Nov 2022 22:49
Operator : CG/JU
Sample : N5592-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

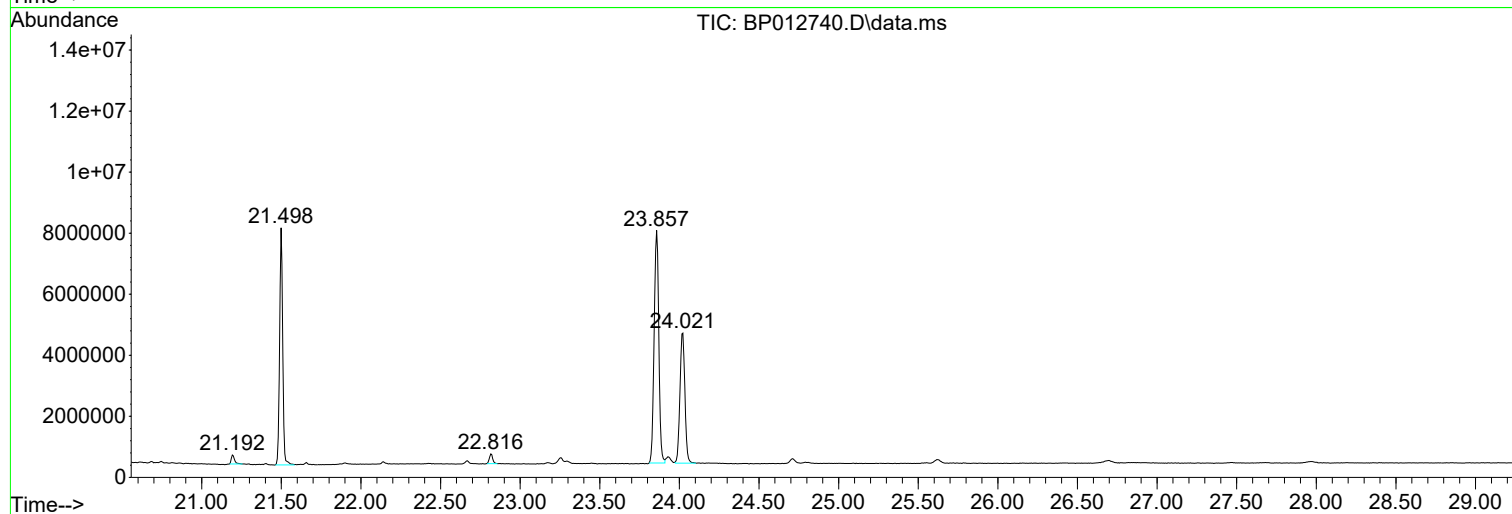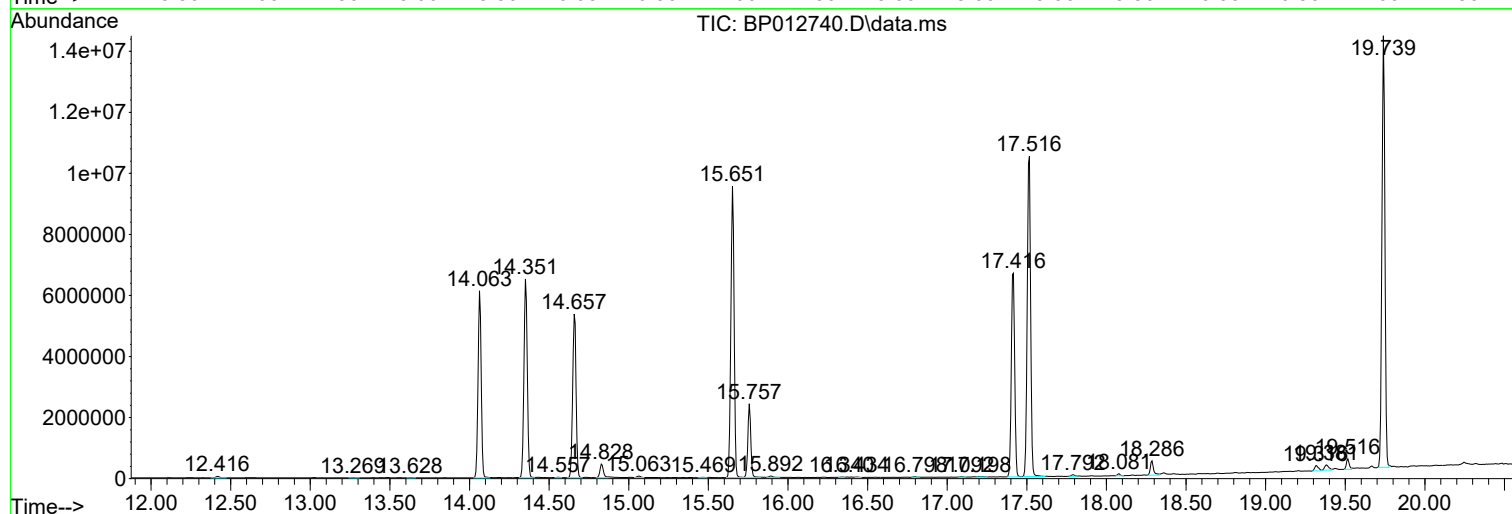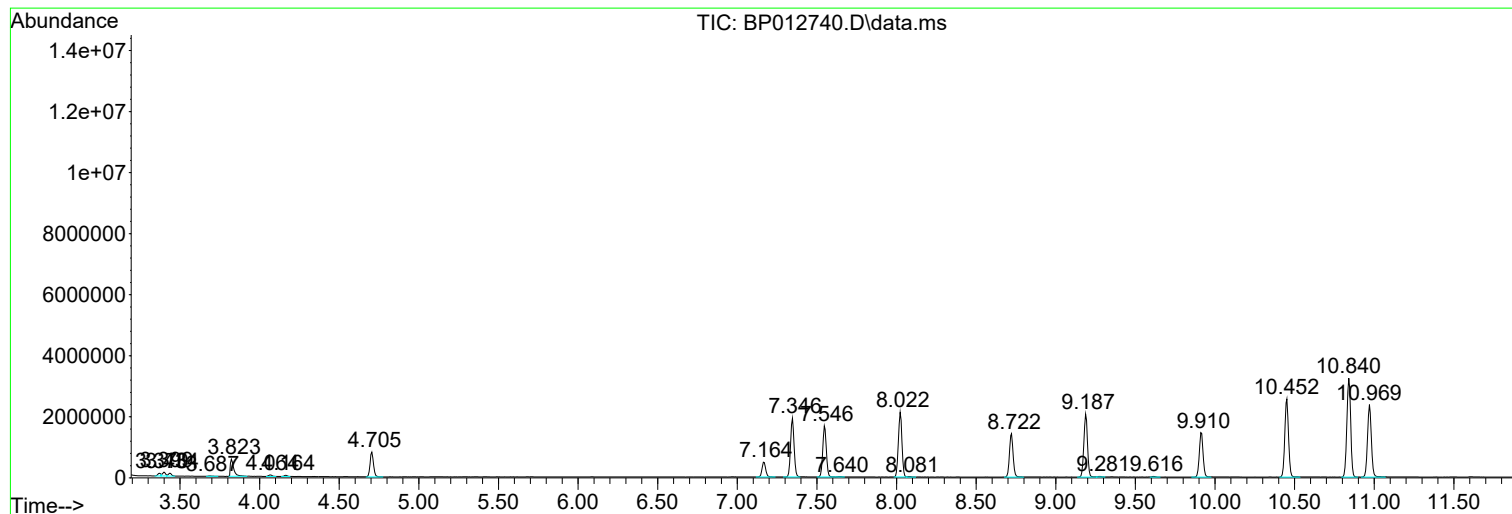

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012740.D
Acq On : 25 Nov 2022 22:49
Operator : CG/JU
Sample : N5592-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012740.D
Acq On : 25 Nov 2022 22:49
Operator : CG/JU
Sample : N5592-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc