

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012741.D
 Acq On : 25 Nov 2022 23:24
 Operator : CG/JU
 Sample : N5592-18
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012741.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	26	31	34	rBV	194785	285498	1.65%	0.197%
2	3.399	34	36	39	rVV	121981	145987	0.84%	0.101%
3	3.434	39	42	50	rVB	92604	133272	0.77%	0.092%
4	3.693	81	86	94	rBV5	13766	30316	0.18%	0.021%
5	3.822	105	108	126	rBV	703974	1053349	6.10%	0.726%
6	4.069	145	150	154	rVB	50385	72631	0.42%	0.050%
7	4.163	162	166	171	rVB	33730	45717	0.26%	0.032%
8	4.705	251	258	272	rVB	1501798	2248170	13.01%	1.549%
9	7.163	670	676	687	rBV	484407	789048	4.57%	0.544%
10	7.346	700	707	716	rBV	2162195	3338730	19.32%	2.300%
11	7.546	734	741	752	rBV	1829277	2884479	16.69%	1.988%
12	8.022	813	822	830	rBV	1850830	2903970	16.80%	2.001%
13	8.722	933	941	949	rBV	1538269	2442740	14.13%	1.683%
14	9.187	1010	1020	1031	rBV	2329474	3720841	21.53%	2.564%
15	9.910	1135	1143	1160	rBV	1650228	2743910	15.88%	1.891%
16	10.451	1226	1235	1246	rBV	2786815	4648121	26.90%	3.203%
17	10.840	1292	1301	1311	rBV	2790741	4581287	26.51%	3.157%
18	10.969	1315	1323	1337	rBV	2621909	4396800	25.44%	3.030%
19	12.416	1562	1569	1575	rBV2	52426	87790	0.51%	0.060%
20	13.269	1706	1714	1719	rBV6	10402	18219	0.11%	0.013%
21	13.551	1756	1762	1769	rBV	31174	51702	0.30%	0.036%
22	13.628	1769	1775	1781	rVB3	12124	21701	0.13%	0.015%
23	14.063	1841	1849	1863	rBV	6308041	8541834	49.43%	5.886%
24	14.351	1890	1898	1912	rBV2	7081037	10356639	59.93%	7.136%
25	14.657	1942	1950	1959	rBV	4496596	6681574	38.66%	4.604%
26	14.828	1973	1979	1986	rBV	372332	558773	3.23%	0.385%
27	15.063	2014	2019	2025	rVB4	34274	55803	0.32%	0.038%
28	15.457	2079	2086	2091	rBV4	10323	20061	0.12%	0.014%
29	15.651	2112	2119	2130	rBV	9257289	13205728	76.41%	9.099%
30	15.757	2130	2137	2152	rVV	2270576	3002367	17.37%	2.069%
31	15.892	2156	2160	2167	rVB	42994	69367	0.40%	0.048%
32	16.222	2213	2216	2221	rVB4	11690	18788	0.11%	0.013%
33	16.439	2248	2253	2260	rVB7	12586	22973	0.13%	0.016%
34	17.086	2356	2363	2368	rBV6	14122	24753	0.14%	0.017%
35	17.416	2411	2419	2428	rBV	5193437	7858722	45.47%	5.415%
36	17.510	2429	2435	2453	rVB2	10246280	15184266	87.86%	10.462%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012741.D
 Acq On : 25 Nov 2022 23:24
 Operator : CG/JU
 Sample : N5592-18
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	17.792	2478	2483	2488	rBV4	20337	31277	0.18%	0.022%
38	18.075	2528	2531	2535	rVB4	15302	19366	0.11%	0.013%
39	18.280	2562	2566	2574	rBV	216879	301343	1.74%	0.208%
40	18.363	2576	2580	2586	rVB3	35186	59743	0.35%	0.041%
41	19.316	2737	2742	2748	rBV3	125504	193032	1.12%	0.133%
42	19.380	2749	2753	2760	rBV	123036	201349	1.17%	0.139%
43	19.516	2772	2776	2783	rBV2	163222	223718	1.29%	0.154%
44	19.669	2798	2802	2807	rBV5	21172	28534	0.17%	0.020%
45	19.739	2808	2814	2828	rVV	13026628	17281690	100.00%	11.908%
46	19.957	2847	2851	2859	rBV	197211	245777	1.42%	0.169%
47	21.192	3058	3061	3065	rBV3	107178	150521	0.87%	0.104%
48	21.498	3107	3113	3119	rBV	5415157	7252547	41.97%	4.997%
49	23.857	3506	3514	3522	rBV2	5632609	11377645	65.84%	7.840%
50	24.015	3534	3541	3553	rVB2	2653828	5518543	31.93%	3.802%




Sum of corrected areas: 145131011

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012741.D
Acq On : 25 Nov 2022 23:24
Operator : CG/JU
Sample : N5592-18
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

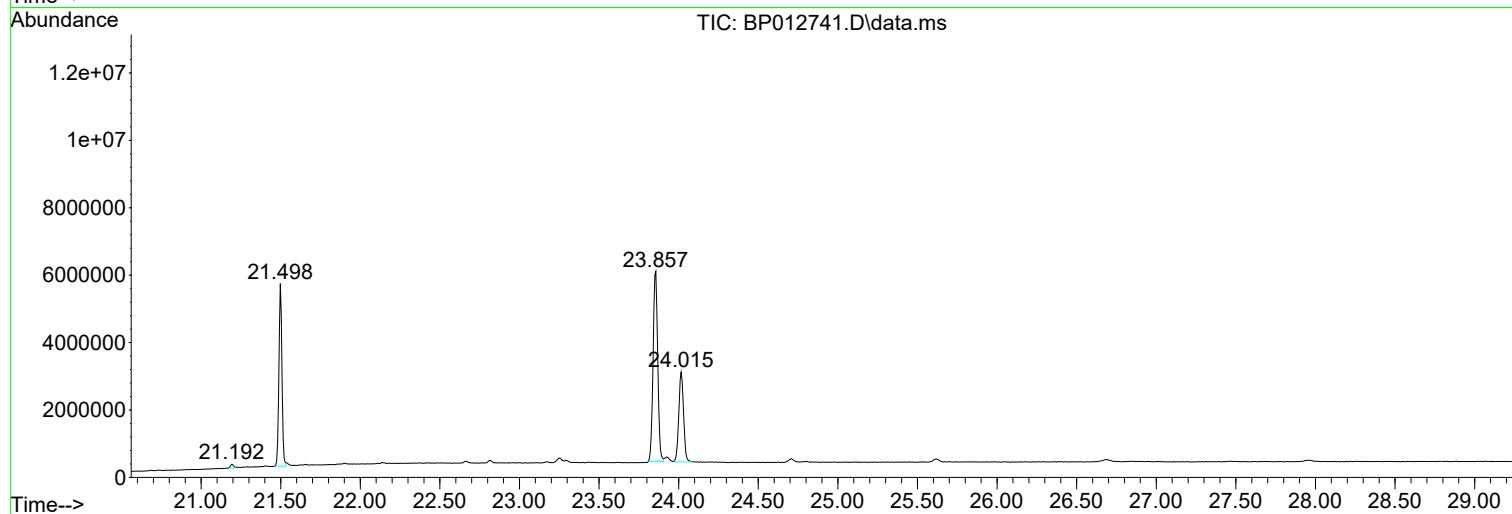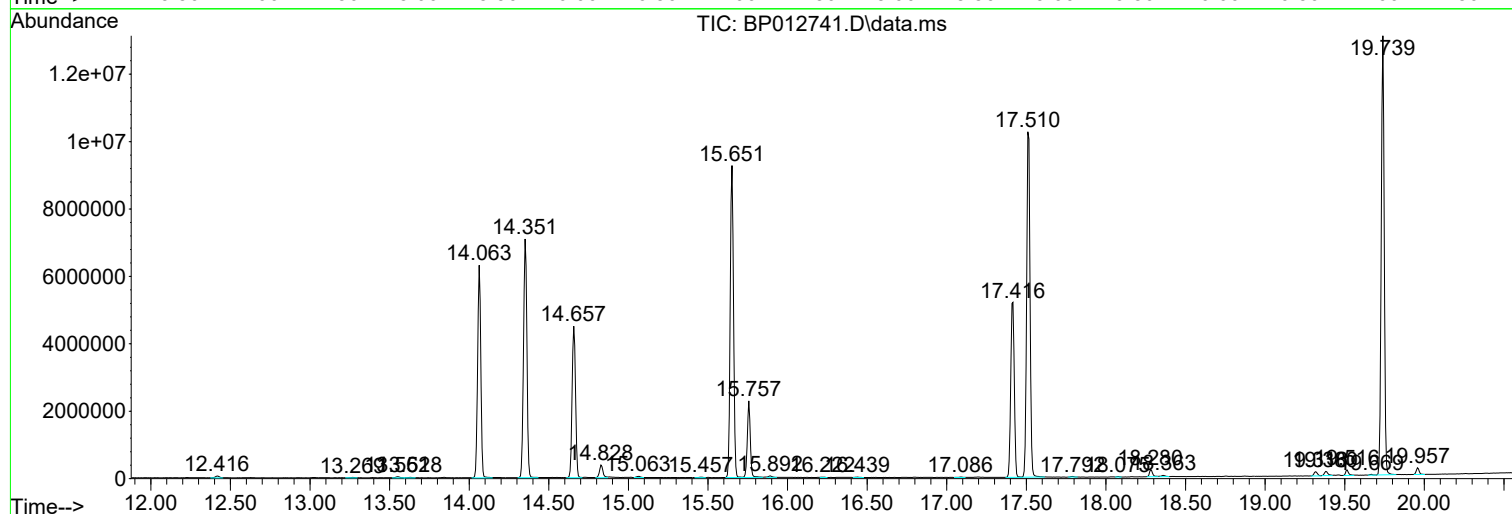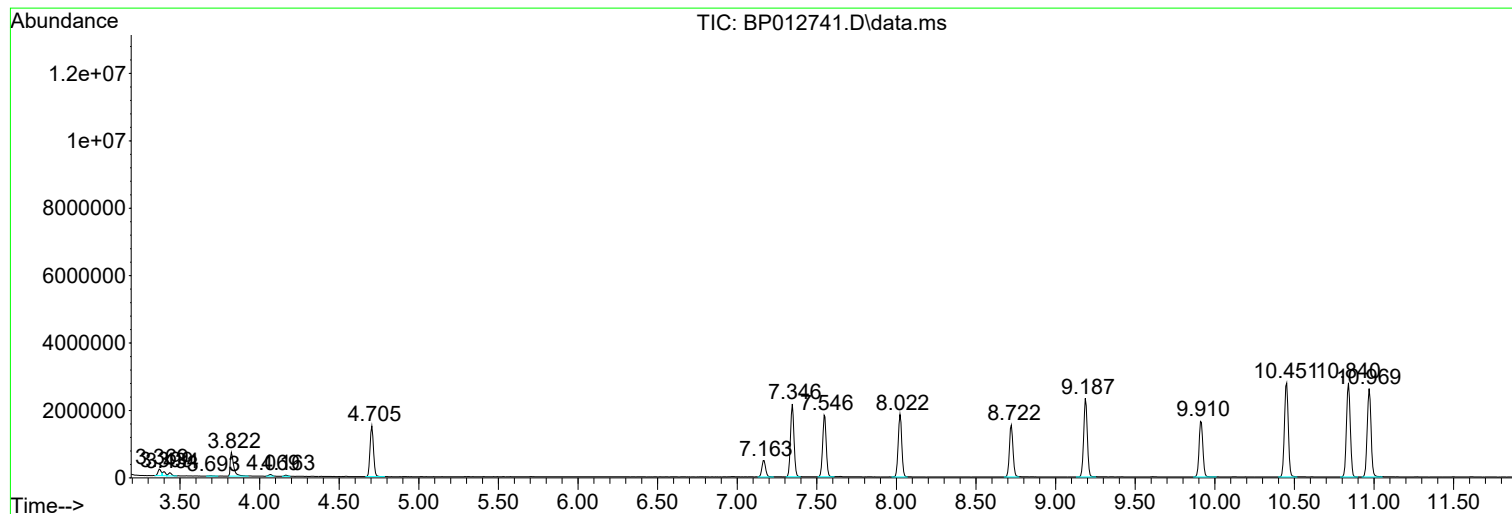

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012741.D
Acq On : 25 Nov 2022 23:24
Operator : CG/JU
Sample : N5592-18
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012741.D
Acq On : 25 Nov 2022 23:24
Operator : CG/JU
Sample : N5592-18
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc