

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012742.D
 Acq On : 25 Nov 2022 23:58
 Operator : CG/JU
 Sample : N5592-19
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012742.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	26	31	34	rBV	230856	336950	2.33%	0.259%
2	3.399	34	36	39	rVV	127859	153753	1.06%	0.118%
3	3.434	39	42	49	rVB	99651	140097	0.97%	0.108%
4	3.699	82	87	92	rBV7	9168	15925	0.11%	0.012%
5	3.822	105	108	128	rBV	655886	959278	6.64%	0.737%
6	4.069	145	150	155	rVB	56113	86897	0.60%	0.067%
7	4.164	162	166	173	rVB	36322	56876	0.39%	0.044%
8	4.705	251	258	273	rVB	1517533	2235341	15.47%	1.718%
9	7.163	668	676	688	rBV	499909	828447	5.73%	0.637%
10	7.346	700	707	718	rBV	2153183	3307299	22.89%	2.542%
11	7.546	733	741	751	rBV	1861481	2970494	20.56%	2.283%
12	7.646	753	758	764	rVB5	12455	25189	0.17%	0.019%
13	8.022	814	822	829	rBV	1779154	2790163	19.31%	2.144%
14	8.081	829	832	838	rVB4	10783	19272	0.13%	0.015%
15	8.722	933	941	951	rBV	1563416	2488482	17.22%	1.913%
16	9.187	1012	1020	1033	rBV	2311741	3625646	25.09%	2.787%
17	9.610	1088	1092	1097	rVB4	11668	18088	0.13%	0.014%
18	9.910	1135	1143	1160	rBV	1674535	2761304	19.11%	2.122%
19	10.451	1226	1235	1252	rBV	2829389	4717703	32.65%	3.626%
20	10.840	1292	1301	1313	rBV	2600888	4335737	30.01%	3.332%
21	10.969	1315	1323	1337	rBV	2554078	4288519	29.68%	3.296%
22	12.422	1562	1570	1577	rBV	51330	88172	0.61%	0.068%
23	13.269	1709	1714	1721	rVB8	10157	20594	0.14%	0.016%
24	13.551	1756	1762	1769	rBV	23649	39089	0.27%	0.030%
25	13.628	1771	1775	1779	rVV3	10586	15369	0.11%	0.012%
26	14.063	1842	1849	1865	rBV	5817146	7928197	54.87%	6.094%
27	14.351	1891	1898	1911	rBV	6893184	9852335	68.19%	7.572%
28	14.657	1942	1950	1958	rBV	4196326	6131646	42.44%	4.713%
29	14.828	1973	1979	1986	rBV	319232	485765	3.36%	0.373%
30	15.063	2014	2019	2027	rVB6	31113	49043	0.34%	0.038%
31	15.651	2112	2119	2130	rBV	8926122	12318450	85.26%	9.468%
32	15.757	2130	2137	2153	rVV	2077324	2664246	18.44%	2.048%
33	15.892	2155	2160	2165	rVB2	38734	62805	0.43%	0.048%
34	16.433	2249	2252	2258	rVB7	12025	17777	0.12%	0.014%
35	16.798	2310	2314	2320	rBV8	10960	17408	0.12%	0.013%
36	17.092	2360	2364	2369	rVB6	11541	17558	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012742.D
Acq On : 25 Nov 2022 23:58
Operator : CG/JU
Sample : N5592-19
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION

37	17.416	2412	2419	2428	rBV	4748973	6945579	48.07%	5.338%
38	17.510	2428	2435	2453	rVV	9179163	13472363	93.25%	10.355%
39	18.280	2561	2566	2576	rBV	269447	397656	2.75%	0.306%
40	18.357	2576	2579	2585	rVB3	34319	51338	0.36%	0.039%
41	19.316	2738	2742	2748	rBV2	122183	171835	1.19%	0.132%
42	19.380	2749	2753	2760	rBV	107294	176130	1.22%	0.135%
43	19.510	2772	2775	2783	rBV	176085	239289	1.66%	0.184%
44	19.739	2808	2814	2831	rBV	11101138	14448326	100.00%	11.105%
45	21.192	3058	3061	3069	rBV2	170085	219484	1.52%	0.169%
46	21.498	3107	3113	3125	rBV	4004467	5424348	37.54%	4.169%
47	23.851	3505	3513	3523	rBV2	4162151	8585746	59.42%	6.599%
48	24.015	3534	3541	3554	rVB2	1995150	4106244	28.42%	3.156%




Sum of corrected areas: 130108252

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012742.D
Acq On : 25 Nov 2022 23:58
Operator : CG/JU
Sample : N5592-19
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

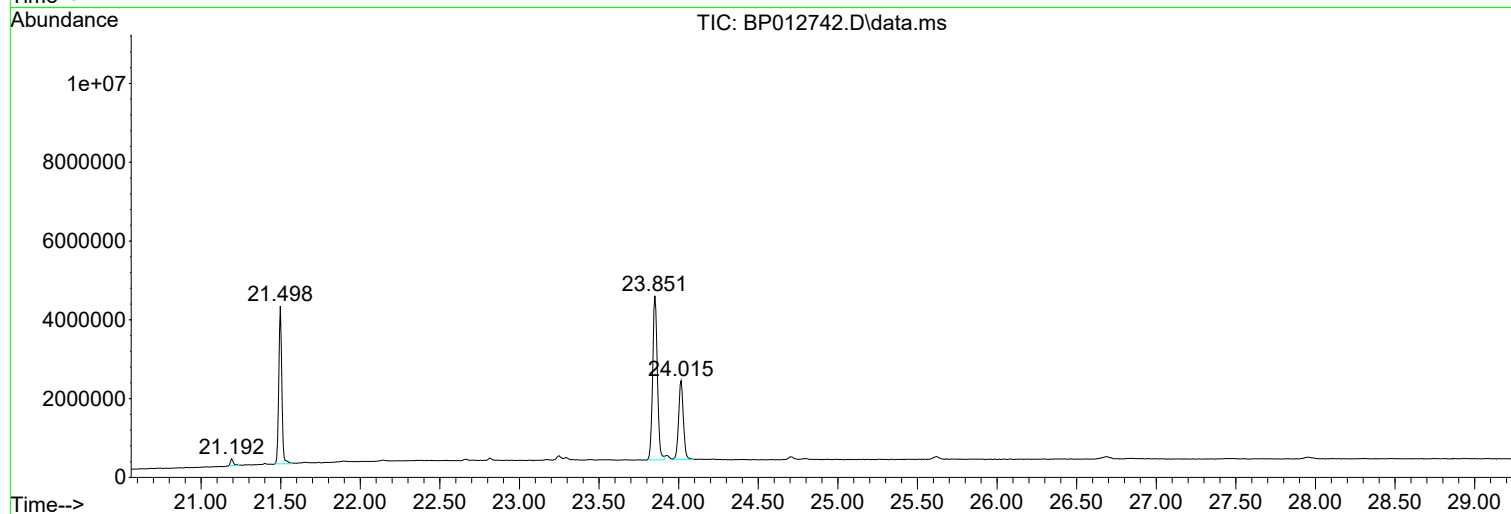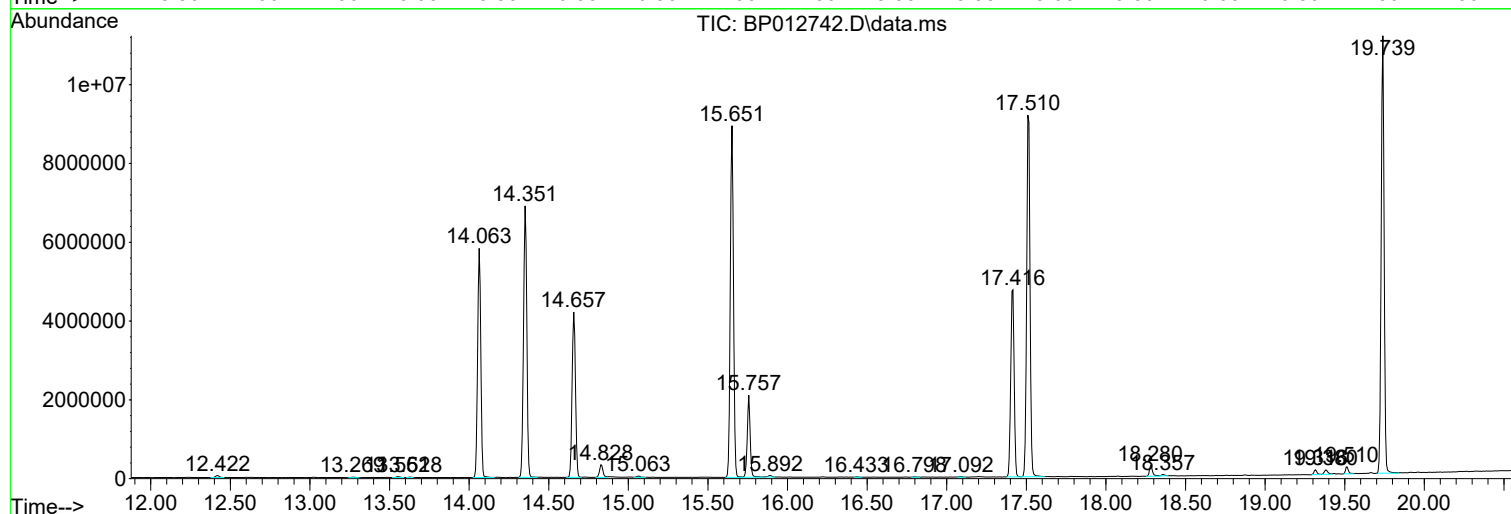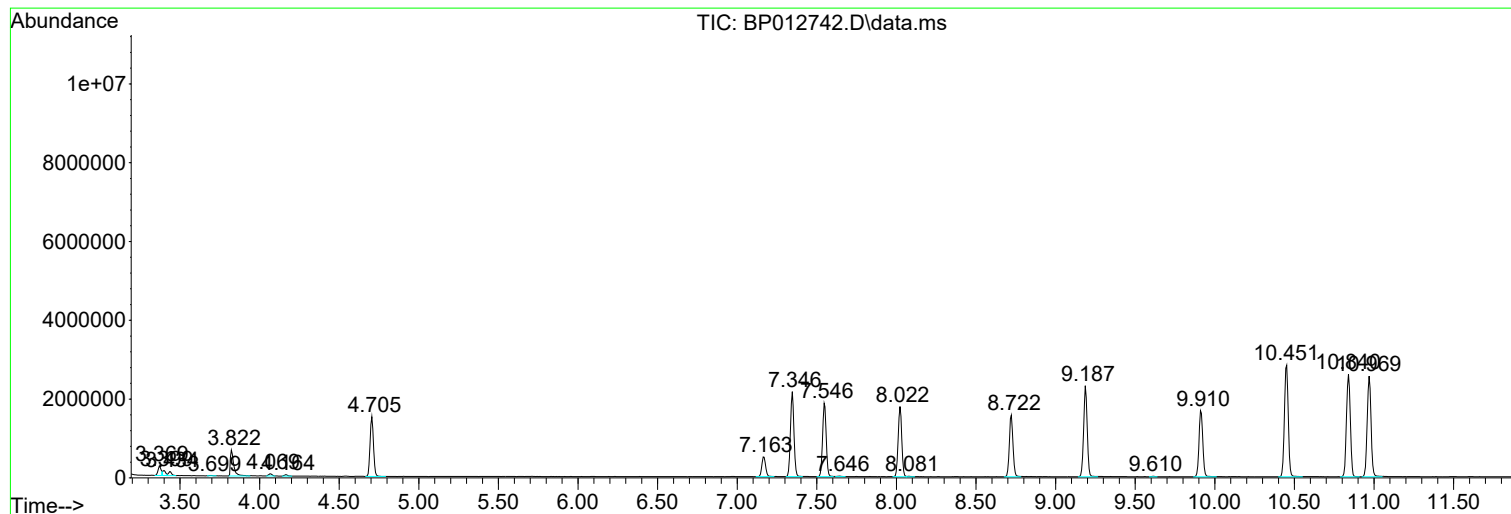

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012742.D
Acq On : 25 Nov 2022 23:58
Operator : CG/JU
Sample : N5592-19
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012742.D
Acq On : 25 Nov 2022 23:58
Operator : CG/JU
Sample : N5592-19
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc