

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012744.D
 Acq On : 26 Nov 2022 01:06
 Operator : CG/JU
 Sample : N5592-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012744.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	26	31	34	rBV	251379	376166	1.83%	0.248%
2	3.399	34	36	40	rVV	140525	174566	0.85%	0.115%
3	3.434	40	42	49	rVB	32282	46010	0.22%	0.030%
4	3.822	105	108	123	rBV	569338	843669	4.10%	0.555%
5	4.069	145	150	155	rVB	48800	77404	0.38%	0.051%
6	4.164	162	166	172	rVB	38451	51079	0.25%	0.034%
7	4.705	251	258	272	rVB	13367228	20553939	100.00%	13.527%
8	7.163	669	676	684	rBV	517701	839824	4.09%	0.553%
9	7.346	700	707	716	rBV	1969566	3078585	14.98%	2.026%
10	7.546	732	741	750	rBV	1726395	2720835	13.24%	1.791%
11	8.022	815	822	830	rBV	1974311	3085270	15.01%	2.030%
12	8.722	933	941	953	rBV	1560747	2504257	12.18%	1.648%
13	9.187	1012	1020	1032	rBV	2152409	3397374	16.53%	2.236%
14	9.610	1086	1092	1099	rVB6	11757	23541	0.11%	0.015%
15	9.910	1132	1143	1157	rBV	1512618	2453936	11.94%	1.615%
16	10.451	1225	1235	1249	rBV	2719807	4532007	22.05%	2.983%
17	10.840	1293	1301	1312	rVB	2961285	4897021	23.83%	3.223%
18	10.969	1315	1323	1336	rBV	1928917	3251138	15.82%	2.140%
19	11.604	1426	1431	1436	rBV5	15435	26154	0.13%	0.017%
20	12.416	1564	1569	1575	rVB2	47838	77526	0.38%	0.051%
21	13.551	1756	1762	1768	rBV5	16666	28130	0.14%	0.019%
22	13.628	1768	1775	1781	rBV4	12564	21972	0.11%	0.014%
23	14.063	1841	1849	1860	rBV	6200905	8460832	41.16%	5.568%
24	14.351	1890	1898	1913	rBV	6902921	9940049	48.36%	6.542%
25	14.657	1943	1950	1959	rBV	4747490	6921971	33.68%	4.555%
26	14.828	1972	1979	1999	rBV	360305	616024	3.00%	0.405%
27	15.063	2013	2019	2024	rBV2	38326	58873	0.29%	0.039%
28	15.651	2112	2119	2126	rBV	9071801	12809955	62.32%	8.430%
29	15.757	2130	2137	2150	rVV	1977079	2605246	12.68%	1.715%
30	15.886	2155	2159	2165	rVB	39730	66273	0.32%	0.044%
31	16.439	2249	2253	2261	rVB6	12146	21477	0.10%	0.014%
32	17.198	2379	2382	2389	rVB2	12730	20954	0.10%	0.014%
33	17.410	2411	2418	2428	rBV	5447986	7830583	38.10%	5.153%
34	17.510	2428	2435	2454	rVV2	9582788	14207445	69.12%	9.350%
35	18.075	2527	2531	2535	rVB	36369	44171	0.21%	0.029%
36	18.280	2562	2566	2573	rBV	175133	237354	1.15%	0.156%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012744.D
Acq On : 26 Nov 2022 01:06
Operator : CG/JU
Sample : N5592-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION

37	18.363	2575	2580	2588	rVB	286143	387539	1.89%	0.255%
38	19.316	2738	2742	2748	rBV2	119563	175908	0.86%	0.116%
39	19.380	2749	2753	2760	rVV	113975	175542	0.85%	0.116%
40	19.510	2772	2775	2788	rBV	126303	166932	0.81%	0.110%
41	19.663	2798	2801	2805	rVB2	26449	30342	0.15%	0.020%
42	19.739	2808	2814	2826	rBV	11393529	14967050	72.82%	9.850%
43	21.498	3107	3113	3124	rBV	4305955	5909775	28.75%	3.889%
44	23.851	3505	3513	3523	rBV2	4228397	8746132	42.55%	5.756%
45	24.015	3534	3541	3553	rVB	2149232	4491431	21.85%	2.956%




Sum of corrected areas: 151952261

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012744.D
Acq On : 26 Nov 2022 01:06
Operator : CG/JU
Sample : N5592-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

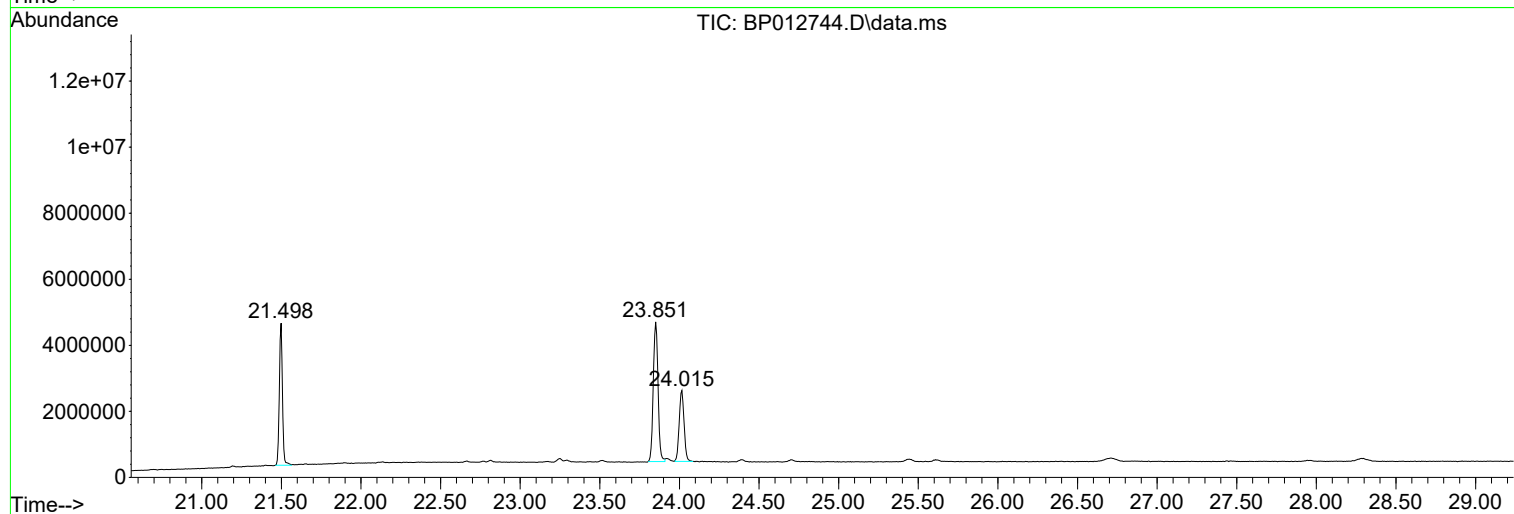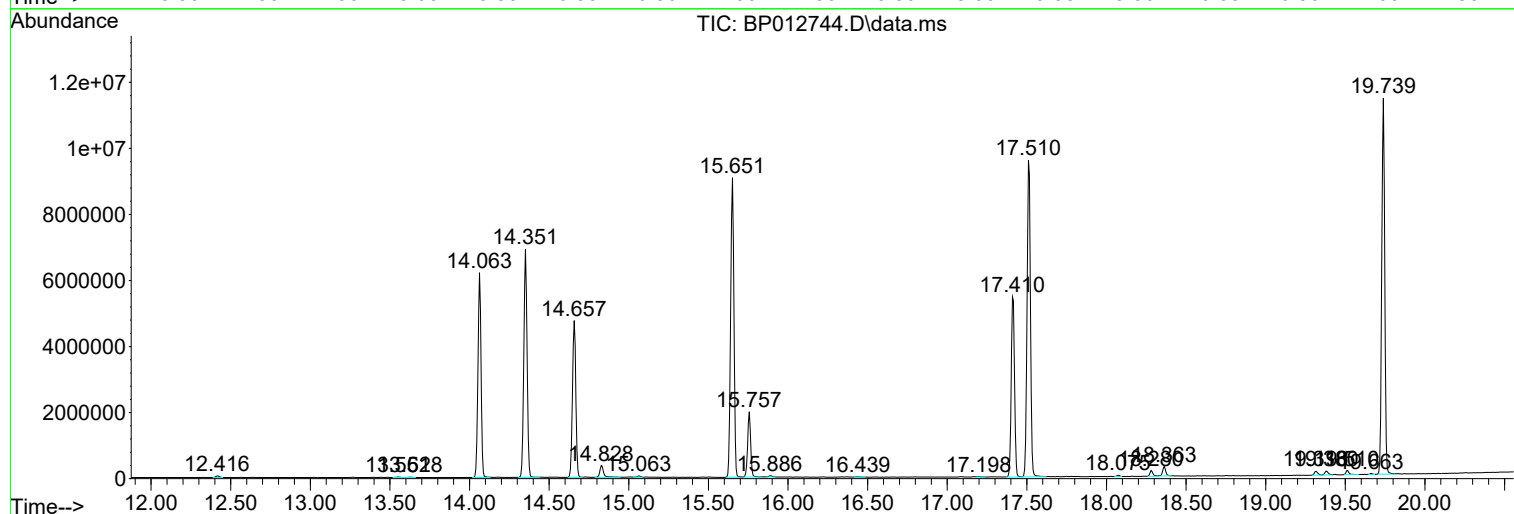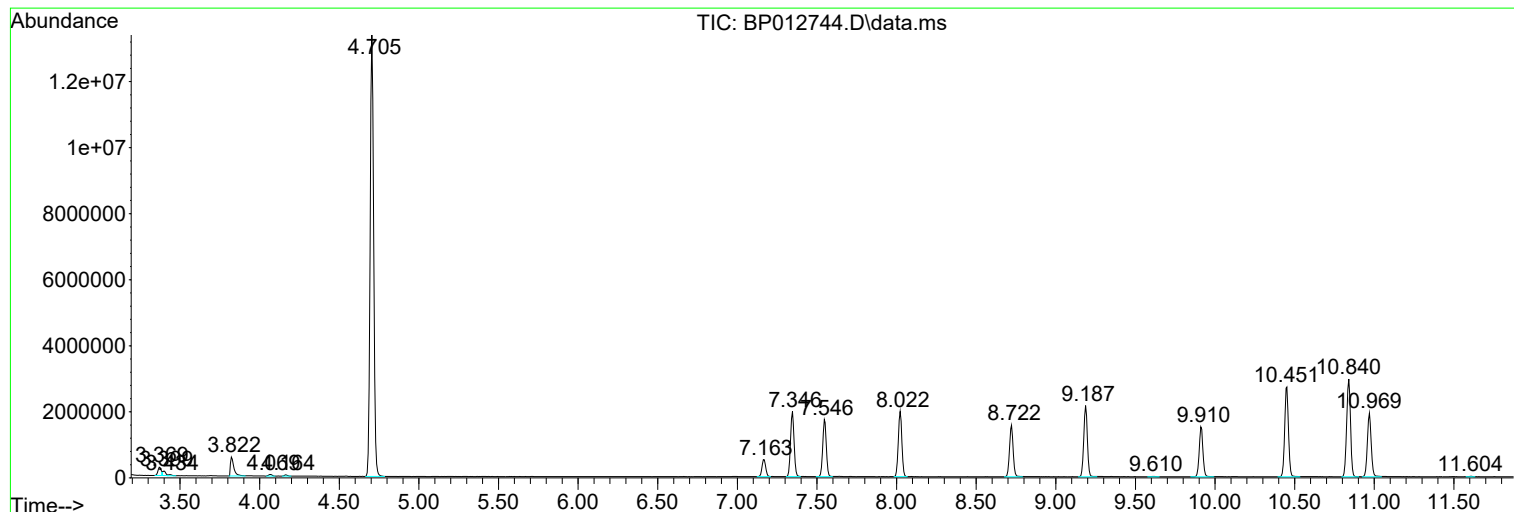

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012744.D
Acq On : 26 Nov 2022 01:06
Operator : CG/JU
Sample : N5592-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012744.D
Acq On : 26 Nov 2022 01:06
Operator : CG/JU
Sample : N5592-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc