

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012745.D
 Acq On : 26 Nov 2022 01:40
 Operator : CG/JU
 Sample : N5592-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012745.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	26	31	34	rBV	274619	395687	1.97%	0.242%
2	3.399	34	36	45	rVB	142271	187827	0.93%	0.115%
3	3.822	104	108	126	rBV	685581	1049008	5.21%	0.640%
4	4.064	145	149	156	rVB	55343	85927	0.43%	0.052%
5	4.164	162	166	174	rVB	37420	52323	0.26%	0.032%
6	4.705	252	258	267	rBV	882709	1336832	6.65%	0.816%
7	7.169	670	677	687	rBV	607272	977834	4.86%	0.597%
8	7.346	700	707	717	rBV	2256164	3475790	17.28%	2.121%
9	7.546	732	741	752	rBV	2014197	3221671	16.02%	1.966%
10	7.646	754	758	764	rVB4	11878	20429	0.10%	0.012%
11	8.022	814	822	830	rBV	1963213	3048192	15.15%	1.860%
12	8.722	932	941	954	rBV	1848665	2925813	14.55%	1.786%
13	9.187	1012	1020	1030	rBV	2449053	3868062	19.23%	2.361%
14	9.910	1135	1143	1152	rBV	1854184	2998979	14.91%	1.830%
15	10.452	1226	1235	1248	rBV	3144325	5250783	26.10%	3.205%
16	10.840	1292	1301	1311	rBV	2836814	4812604	23.93%	2.937%
17	10.969	1315	1323	1338	rBV	2412665	4013462	19.95%	2.450%
18	11.610	1426	1432	1436	rBV6	14066	26965	0.13%	0.016%
19	12.416	1564	1569	1578	rVB	56673	96928	0.48%	0.059%
20	13.628	1769	1775	1782	rBV5	13661	29724	0.15%	0.018%
21	14.063	1842	1849	1864	rBV	7248817	9800111	48.72%	5.982%
22	14.351	1891	1898	1907	rBV2	7903560	11390505	56.63%	6.952%
23	14.657	1942	1950	1958	rBV	4856611	7088951	35.24%	4.327%
24	14.828	1973	1979	1986	rBV	511910	802632	3.99%	0.490%
25	14.892	1986	1990	1996	rVB3	44174	78958	0.39%	0.048%
26	15.063	2014	2019	2025	rVB5	45346	71916	0.36%	0.044%
27	15.651	2111	2119	2128	rBV	10474388	15037086	74.75%	9.178%
28	15.757	2130	2137	2151	rVV	2808987	3647785	18.13%	2.226%
29	15.892	2155	2160	2166	rVB	47224	75409	0.37%	0.046%
30	16.216	2207	2215	2219	rBV6	15238	28429	0.14%	0.017%
31	17.086	2359	2363	2369	rVB6	13260	23268	0.12%	0.014%
32	17.198	2379	2382	2390	rVB2	15024	23170	0.12%	0.014%
33	17.410	2411	2418	2428	rBV	5994421	8524505	42.38%	5.203%
34	17.516	2428	2436	2449	rVV	11848980	17300963	86.01%	10.560%
35	18.075	2528	2531	2536	rBV5	22550	25753	0.13%	0.016%
36	18.281	2561	2566	2575	rBV	280433	403716	2.01%	0.246%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012745.D
 Acq On : 26 Nov 2022 01:40
 Operator : CG/JU
 Sample : N5592-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	18.363	2575	2580	2589	rVV	365899	508311	2.53%	0.310%
38	19.316	2737	2742	2747	rBV	159900	226773	1.13%	0.138%
39	19.380	2748	2753	2760	rBV	155851	255432	1.27%	0.156%
40	19.510	2771	2775	2781	rBV	207876	280298	1.39%	0.171%
41	19.663	2799	2801	2807	rVB3	29442	22502	0.11%	0.014%
42	19.739	2808	2814	2825	rBV	15145205	20115367	100.00%	12.277%
43	21.498	3107	3113	3124	rBV	6141836	8451122	42.01%	5.158%
44	23.857	3505	3514	3522	rBV2	7210670	15001783	74.58%	9.156%
45	24.016	3534	3541	3558	rVB2	3213157	6780470	33.71%	4.138%




Sum of corrected areas: 163840055

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012745.D
Acq On : 26 Nov 2022 01:40
Operator : CG/JU
Sample : N5592-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

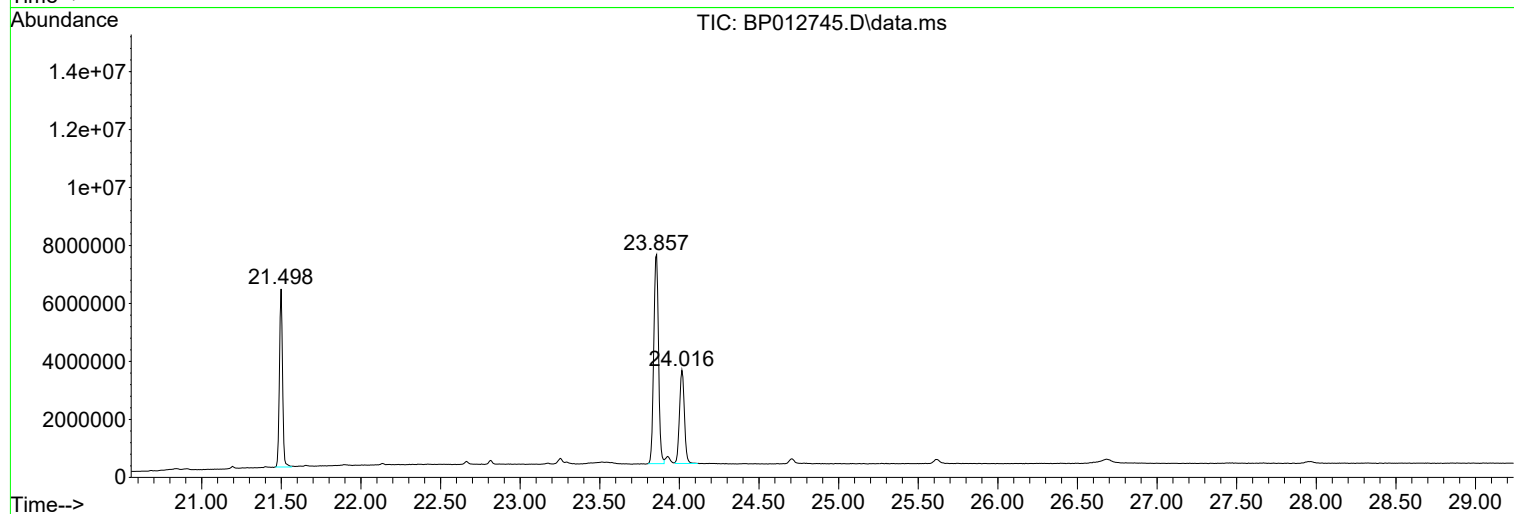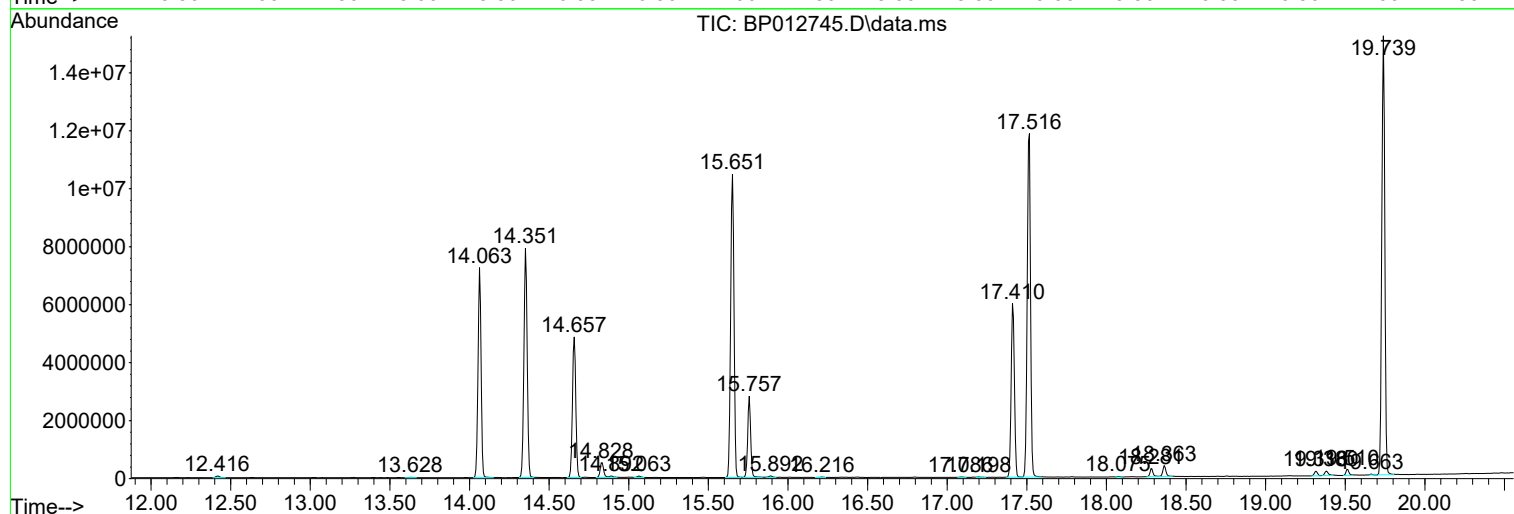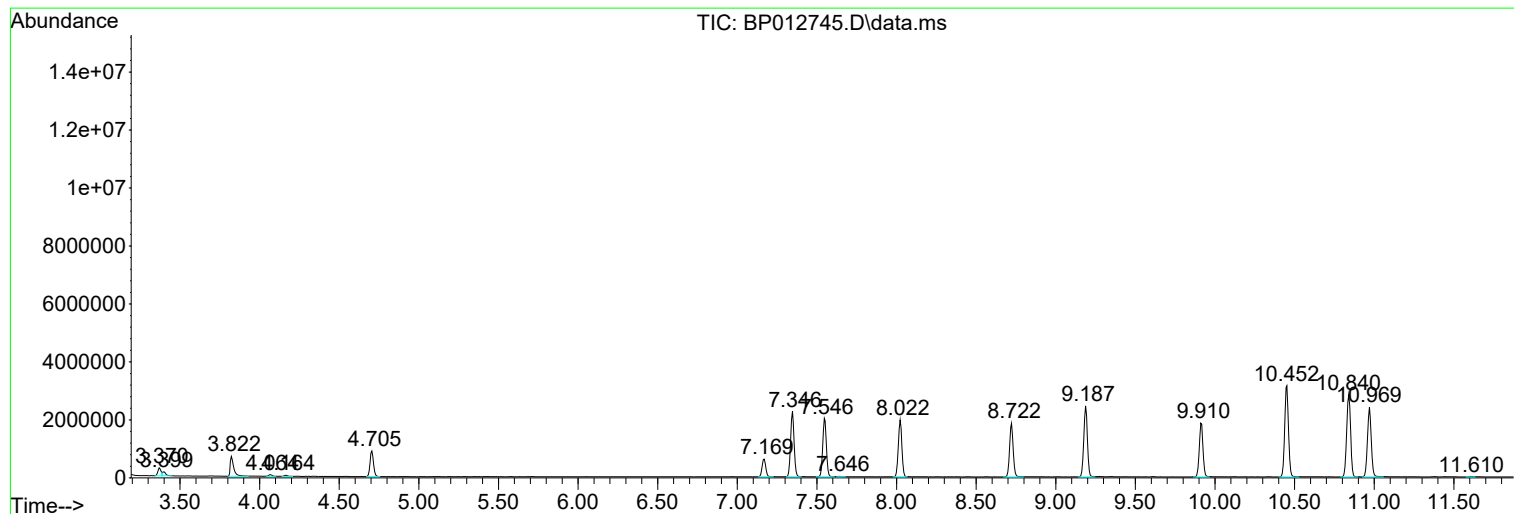

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012745.D
Acq On : 26 Nov 2022 01:40
Operator : CG/JU
Sample : N5592-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012745.D
Acq On : 26 Nov 2022 01:40
Operator : CG/JU
Sample : N5592-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------