

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012746.D
 Acq On : 26 Nov 2022 02:14
 Operator : CG/JU
 Sample : N5592-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012746.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	25	31	39	rBV	3429142	5444369	18.17%	3.044%
2	3.434	39	42	57	rVB	1005850	1312486	4.38%	0.734%
3	3.687	82	85	93	rVB4	16540	31141	0.10%	0.017%
4	3.822	104	108	123	rBV	797079	1187266	3.96%	0.664%
5	4.069	145	150	155	rVB	53605	82315	0.27%	0.046%
6	4.164	161	166	172	rBV	31510	50738	0.17%	0.028%
7	4.705	251	258	273	rBV	18500340	29959184	100.00%	16.751%
8	7.169	670	677	684	rBV	654335	1018198	3.40%	0.569%
9	7.346	699	707	716	rBV	2225783	3423956	11.43%	1.914%
10	7.546	733	741	752	rBV	1982571	3129329	10.45%	1.750%
11	8.022	814	822	830	rBV	1678634	2614446	8.73%	1.462%
12	8.722	933	941	951	rBV	1843103	2906738	9.70%	1.625%
13	9.187	1012	1020	1030	rBV	2382578	3796380	12.67%	2.123%
14	9.910	1136	1143	1159	rBV	1729865	2841401	9.48%	1.589%
15	10.451	1226	1235	1248	rBV	2992257	5026680	16.78%	2.811%
16	10.840	1293	1301	1310	rBV	2486257	4133972	13.80%	2.311%
17	10.969	1315	1323	1342	rBV	2263432	3775796	12.60%	2.111%
18	11.604	1424	1431	1436	rVB4	20957	39785	0.13%	0.022%
19	12.416	1563	1569	1576	rVB	56706	91009	0.30%	0.051%
20	13.269	1707	1714	1721	rVB3	18757	34284	0.11%	0.019%
21	14.063	1842	1849	1859	rBV	6872876	9256794	30.90%	5.176%
22	14.351	1891	1898	1910	rBV	7657783	11048437	36.88%	6.177%
23	14.657	1942	1950	1957	rBV	4129766	5943360	19.84%	3.323%
24	14.828	1973	1979	1993	rBV	508271	795005	2.65%	0.445%
25	15.063	2014	2019	2024	rVB5	42816	63058	0.21%	0.035%
26	15.651	2112	2119	2130	rBV	10044423	14319652	47.80%	8.006%
27	15.757	2130	2137	2148	rBV	2415714	3104404	10.36%	1.736%
28	15.892	2154	2160	2167	rVB2	43866	78733	0.26%	0.044%
29	17.222	2383	2386	2390	rVB4	35118	46522	0.16%	0.026%
30	17.410	2412	2418	2425	rBV	4795859	6894377	23.01%	3.855%
31	17.510	2428	2435	2449	rVV2	10663258	15824128	52.82%	8.848%
32	17.833	2486	2490	2494	rVB4	22776	32966	0.11%	0.018%
33	17.910	2499	2503	2507	rVB3	27022	35588	0.12%	0.020%
34	18.075	2527	2531	2536	rVB3	41765	49148	0.16%	0.027%
35	18.280	2562	2566	2574	rBV	335744	465559	1.55%	0.260%
36	18.357	2576	2579	2585	rVB	104208	147878	0.49%	0.083%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012746.D
 Acq On : 26 Nov 2022 02:14
 Operator : CG/JU
 Sample : N5592-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	19.016	2689	2691	2696	rVB2	46457	57615	0.19%	0.032%
38	19.316	2738	2742	2745	rBV	154213	217382	0.73%	0.122%
39	19.380	2749	2753	2759	rVB	144827	239595	0.80%	0.134%
40	19.510	2772	2775	2780	rBV	212911	277600	0.93%	0.155%
41	19.739	2808	2814	2824	rBV	13003084	17303265	57.76%	9.675%
42	19.910	2840	2843	2849	rBV3	64056	119265	0.40%	0.067%
43	21.192	3057	3061	3069	rBV2	275065	395173	1.32%	0.221%
44	21.498	3107	3113	3123	rBV	4281255	5738797	19.16%	3.209%
45	23.851	3505	3513	3531	rBV2	5425468	11092549	37.03%	6.202%
46	24.015	3534	3541	3559	rVB2	2070859	4405775	14.71%	2.463%




Sum of corrected areas: 178852098

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012746.D
Acq On : 26 Nov 2022 02:14
Operator : CG/JU
Sample : N5592-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

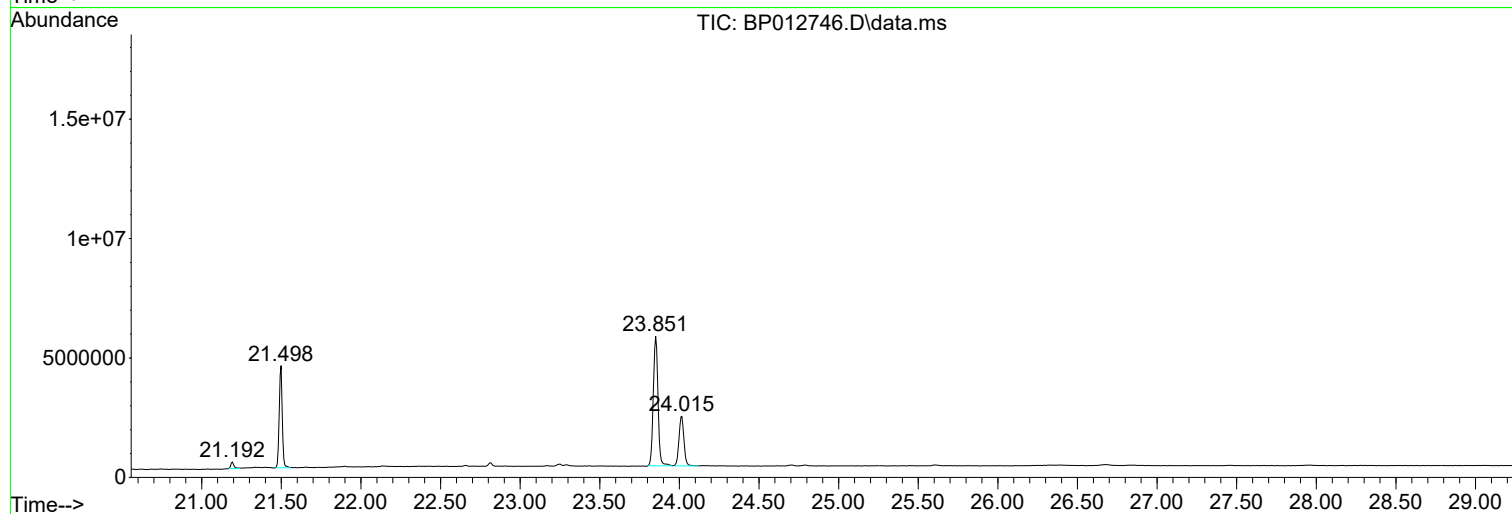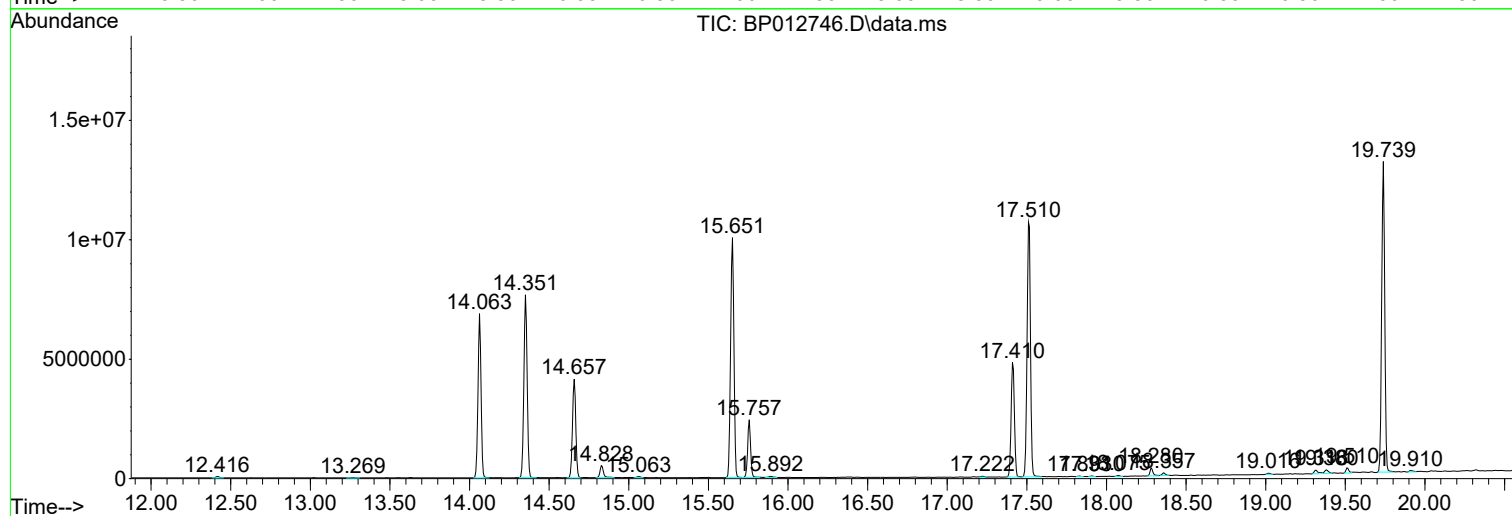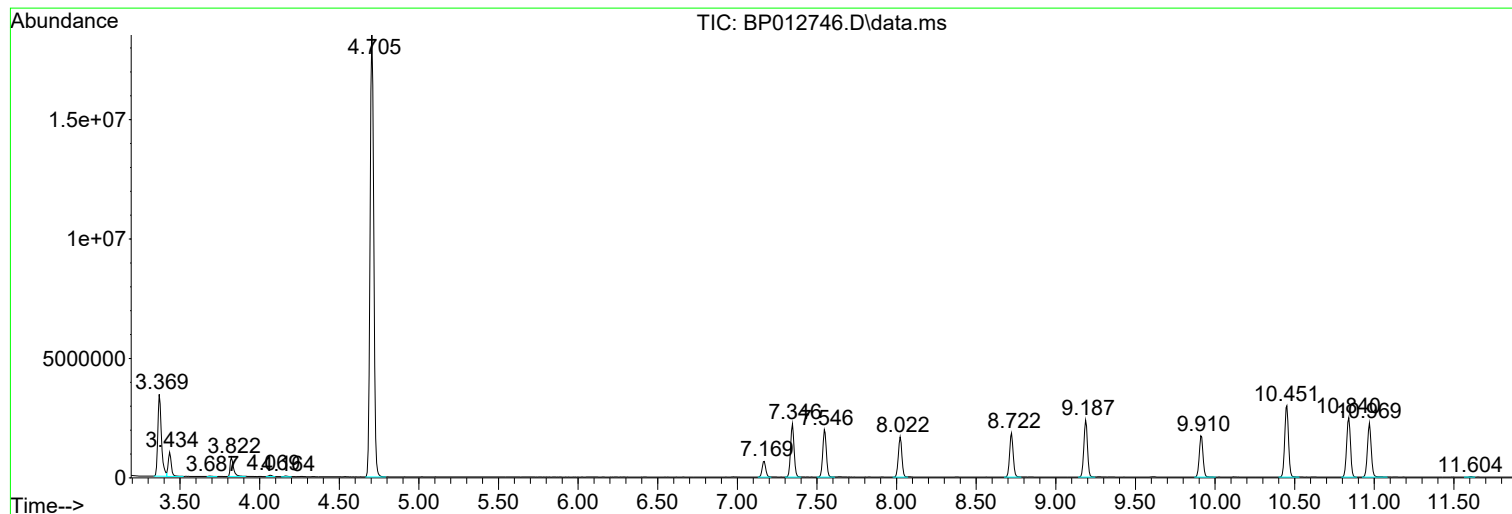

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012746.D
Acq On : 26 Nov 2022 02:14
Operator : CG/JU
Sample : N5592-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012746.D
Acq On : 26 Nov 2022 02:14
Operator : CG/JU
Sample : N5592-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc