

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012750.D
 Acq On : 26 Nov 2022 05:05
 Operator : CG/JU
 Sample : PB149119BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK119

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012750.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	47	rVB	171641	231744	1.54%	0.153%
2	3.822	104	108	135	rBV	2045146	3172050	21.12%	2.100%
3	4.164	161	166	173	rBV	41185	63069	0.42%	0.042%
4	7.169	668	677	689	rBV	2388669	3740909	24.90%	2.476%
5	7.346	700	707	720	rVB	2100879	3259559	21.70%	2.158%
6	7.546	734	741	758	rBV	2408004	3770583	25.10%	2.496%
7	8.022	814	822	832	rBV	2222741	3478677	23.16%	2.303%
8	8.722	933	941	952	rBV	3016599	4837373	32.20%	3.202%
9	9.187	1012	1020	1032	rBV	2254665	3539442	23.56%	2.343%
10	9.910	1135	1143	1152	rBV	1779250	2855849	19.01%	1.890%
11	10.451	1227	1235	1249	rBV	2995491	5047804	33.61%	3.341%
12	10.840	1292	1301	1312	rBV	3238205	5432688	36.17%	3.596%
13	10.969	1315	1323	1335	rBV	3065097	5196237	34.59%	3.440%
14	12.416	1563	1569	1575	rBV2	49667	85890	0.57%	0.057%
15	13.551	1756	1762	1770	rBV3	22481	39192	0.26%	0.026%
16	13.628	1770	1775	1781	rVB4	11972	19699	0.13%	0.013%
17	14.063	1842	1849	1859	rBV	6040358	8221028	54.73%	5.442%
18	14.351	1890	1898	1911	rBV	6860984	9854449	65.61%	6.523%
19	14.657	1943	1950	1958	rBV	5476267	7859654	52.33%	5.203%
20	14.834	1973	1980	2005	rBV	2421026	3469454	23.10%	2.297%
21	15.063	2015	2019	2023	rVB2	15935	19128	0.13%	0.013%
22	15.651	2111	2119	2130	rBV	8719484	12438437	82.81%	8.233%
23	15.757	2130	2137	2151	rVV	2135180	2847792	18.96%	1.885%
24	15.886	2155	2159	2167	rVB	40357	65431	0.44%	0.043%
25	16.433	2248	2252	2260	rVB	9140	17200	0.11%	0.011%
26	17.086	2359	2363	2370	rVB6	9947	15663	0.10%	0.010%
27	17.198	2378	2382	2387	rBV3	13181	20908	0.14%	0.014%
28	17.410	2411	2418	2428	rBV	6550406	9223466	61.40%	6.105%
29	17.510	2428	2435	2453	rVV2	9479403	13591410	90.48%	8.997%
30	18.280	2562	2566	2574	rBV7	14924	29221	0.19%	0.019%
31	19.316	2737	2742	2746	rBV	101274	137481	0.92%	0.091%
32	19.380	2749	2753	2759	rVV	94495	128292	0.85%	0.085%
33	19.739	2807	2814	2825	rBV	11283524	15020732	100.00%	9.943%
34	21.498	3107	3113	3123	rBV	5704139	7905972	52.63%	5.233%
35	23.851	3505	3513	3522	rBV2	4592852	9344079	62.21%	6.185%
36	24.010	3533	3540	3556	rVB2	2894485	6093151	40.56%	4.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012750.D
Acq On : 26 Nov 2022 05:05
Operator : CG/JU
Sample : PB149119BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK119

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION




Sum of corrected areas: 151073713

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012750.D
Acq On : 26 Nov 2022 05:05
Operator : CG/JU
Sample : PB149119BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK119

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

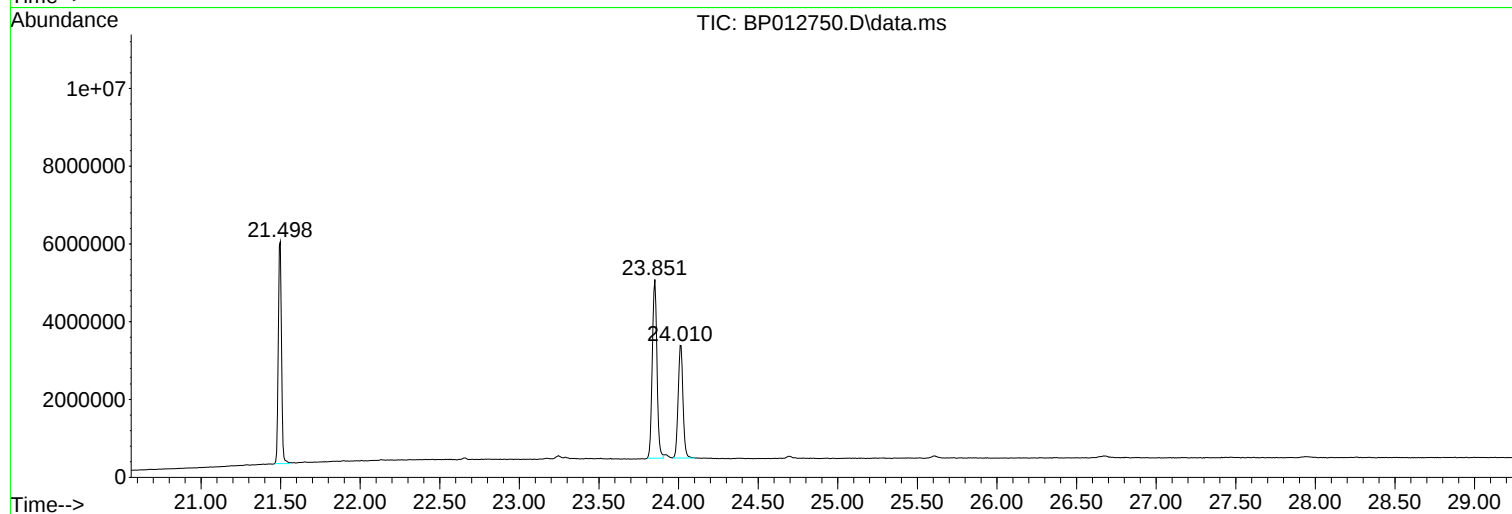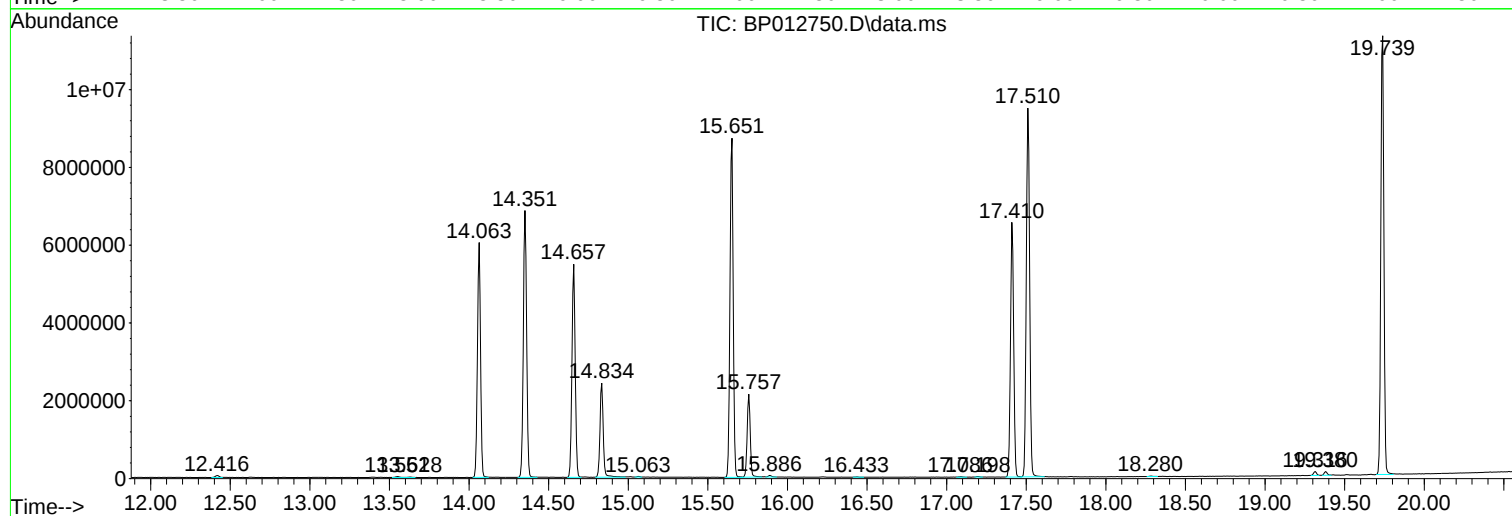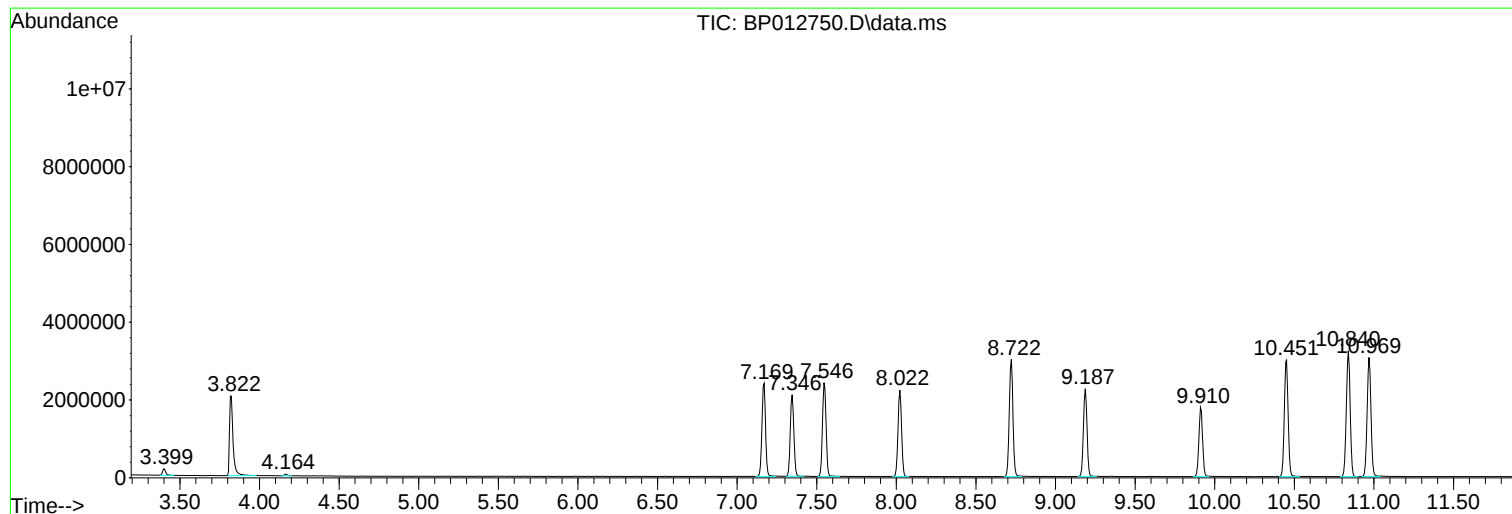

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012750.D
Acq On : 26 Nov 2022 05:05
Operator : CG/JU
Sample : PB149119BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK119

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012750.D
Acq On : 26 Nov 2022 05:05
Operator : CG/JU
Sample : PB149119BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK119

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc