

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012755.D
 Acq On : 26 Nov 2022 07:55
 Operator : CG/JU
 Sample : N5603-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012755.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	50	rVB	129406	201369	1.52%	0.146%
2	3.681	81	84	92	rBV	44895	63989	0.48%	0.046%
3	3.822	104	108	129	rBV	873870	1273625	9.63%	0.923%
4	4.063	145	149	156	rVB	70045	104310	0.79%	0.076%
5	4.163	162	166	172	rVB	41114	56637	0.43%	0.041%
6	4.540	227	230	235	rVB7	11872	16033	0.12%	0.012%
7	5.105	320	326	332	rBV	32126	51424	0.39%	0.037%
8	5.281	351	356	363	rVB	35305	53723	0.41%	0.039%
9	7.163	668	676	688	rBV	770976	1239631	9.37%	0.898%
10	7.346	698	707	716	rBV	2221535	3447248	26.07%	2.497%
11	7.546	733	741	753	rBV	2226322	3432922	25.96%	2.487%
12	7.640	753	757	762	rVB7	11212	21197	0.16%	0.015%
13	8.022	813	822	829	rBV	2195067	3479037	26.31%	2.520%
14	8.722	933	941	952	rBV	1985866	3225338	24.39%	2.336%
15	9.187	1013	1020	1030	rBV	2372629	3802543	28.75%	2.754%
16	9.275	1030	1035	1042	rVV6	16507	36024	0.27%	0.026%
17	9.610	1086	1092	1099	rVB5	17226	33178	0.25%	0.024%
18	9.910	1135	1143	1153	rBV	1850451	2963197	22.41%	2.146%
19	10.445	1226	1234	1251	rBV	3114158	5194735	39.28%	3.763%
20	10.616	1257	1263	1272	rVB	22387	47604	0.36%	0.034%
21	10.840	1292	1301	1308	rBV	3179661	5322110	40.24%	3.855%
22	10.969	1315	1323	1344	rBV	2332001	4010215	30.32%	2.905%
23	11.263	1368	1373	1379	rVB5	13013	24160	0.18%	0.018%
24	11.404	1392	1397	1403	rVB6	24441	45362	0.34%	0.033%
25	11.604	1425	1431	1435	rBV6	16073	30203	0.23%	0.022%
26	11.963	1487	1492	1500	rVB6	6682	17272	0.13%	0.013%
27	12.110	1507	1517	1522	rBV6	5925	17833	0.13%	0.013%
28	12.416	1562	1569	1576	rVB	54051	93785	0.71%	0.068%
29	13.269	1707	1714	1721	rVB	13984	32613	0.25%	0.024%
30	13.551	1757	1762	1767	rVB8	9137	16686	0.13%	0.012%
31	13.628	1767	1775	1781	rBV7	17749	43363	0.33%	0.031%
32	14.063	1842	1849	1859	rBV	5811100	8097596	61.23%	5.865%
33	14.181	1866	1869	1877	rVB10	13062	31590	0.24%	0.023%
34	14.298	1885	1889	1891	rBV3	30842	43759	0.33%	0.032%
35	14.351	1891	1898	1907	rVB	6845268	10014106	75.72%	7.254%
36	14.557	1930	1933	1940	rVB4	17449	28594	0.22%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012755.D
 Acq On : 26 Nov 2022 07:55
 Operator : CG/JU
 Sample : N5603-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	14.657	1943	1950	1958	rVV	4996767	7156210	54.11%	5.184%
38	14.728	1959	1962	1968	rVB7	14273	22364	0.17%	0.016%
39	14.833	1973	1980	1995	rBV	470406	801534	6.06%	0.581%
40	15.063	2016	2019	2023	rVB5	17883	22085	0.17%	0.016%
41	15.286	2053	2057	2064	rBV8	13494	32614	0.25%	0.024%
42	15.457	2082	2086	2087	rBV2	18723	23082	0.17%	0.017%
43	15.651	2112	2119	2130	rBV	8457577	12472436	94.31%	9.034%
44	15.757	2131	2137	2150	rVV	2012804	2762078	20.89%	2.001%
45	15.886	2156	2159	2166	rVB4	36230	57944	0.44%	0.042%
46	17.410	2412	2418	2428	rBV	5468929	7589074	57.39%	5.497%
47	17.510	2428	2435	2444	rBV	9019662	12831065	97.02%	9.294%
48	17.774	2477	2480	2488	rVB	72816	105136	0.80%	0.076%
49	18.280	2562	2566	2574	rBV	229721	337617	2.55%	0.245%
50	19.316	2738	2742	2746	rBV	105120	140880	1.07%	0.102%
51	19.380	2749	2753	2759	rVV	101722	162074	1.23%	0.117%
52	19.510	2772	2775	2780	rBV	190716	238806	1.81%	0.173%
53	19.733	2807	2813	2827	rBV	9611972	13224546	100.00%	9.579%
54	21.192	3058	3061	3068	rBV3	104898	136701	1.03%	0.099%
55	21.492	3107	3112	3126	rBV	4509479	6135202	46.39%	4.444%
56	23.845	3505	3512	3522	rBV2	5417373	10977647	83.01%	7.952%
57	24.009	3533	3540	3556	rVB2	3003124	6214521	46.99%	4.501%




Sum of corrected areas: 138056627

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012755.D
Acq On : 26 Nov 2022 07:55
Operator : CG/JU
Sample : N5603-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

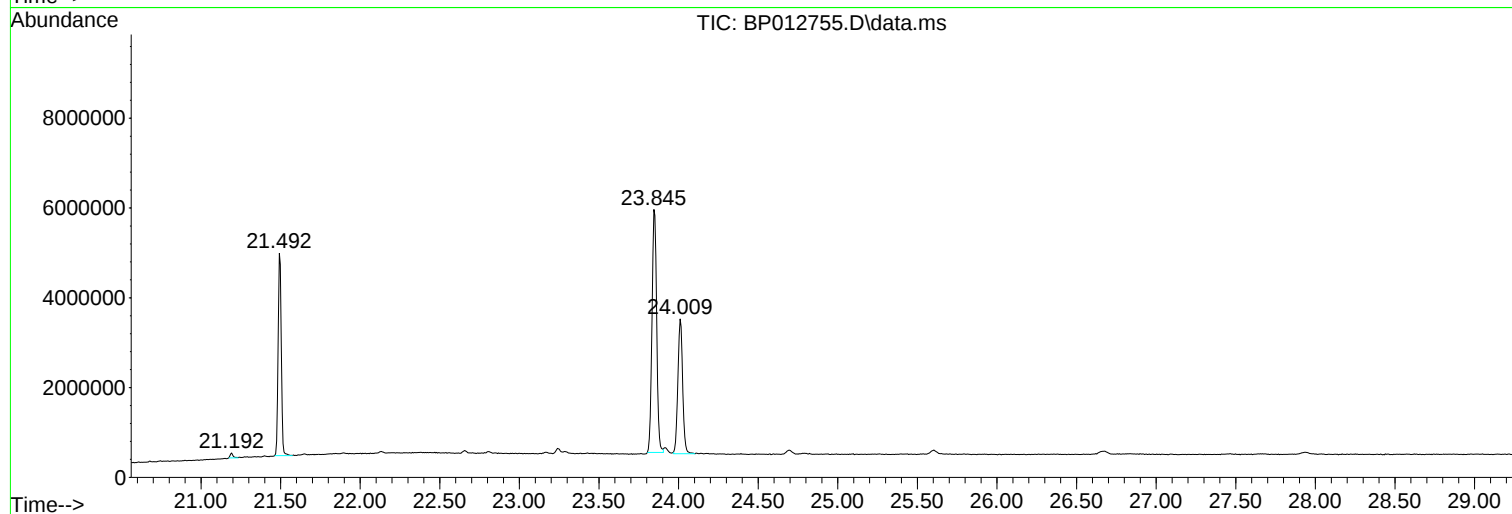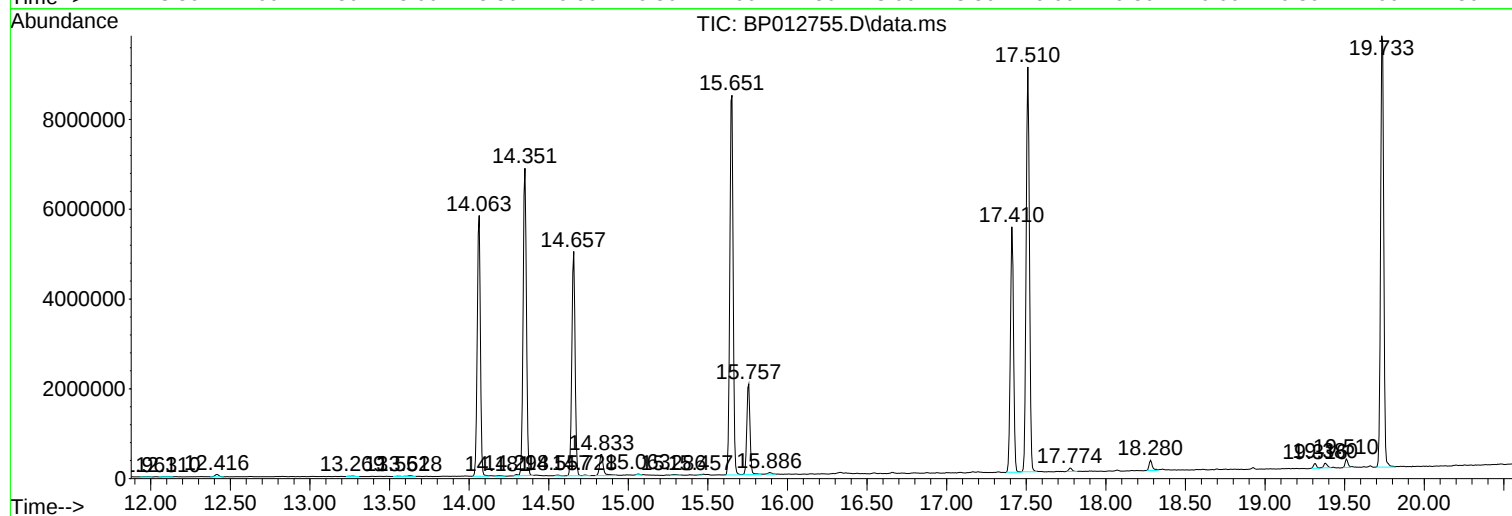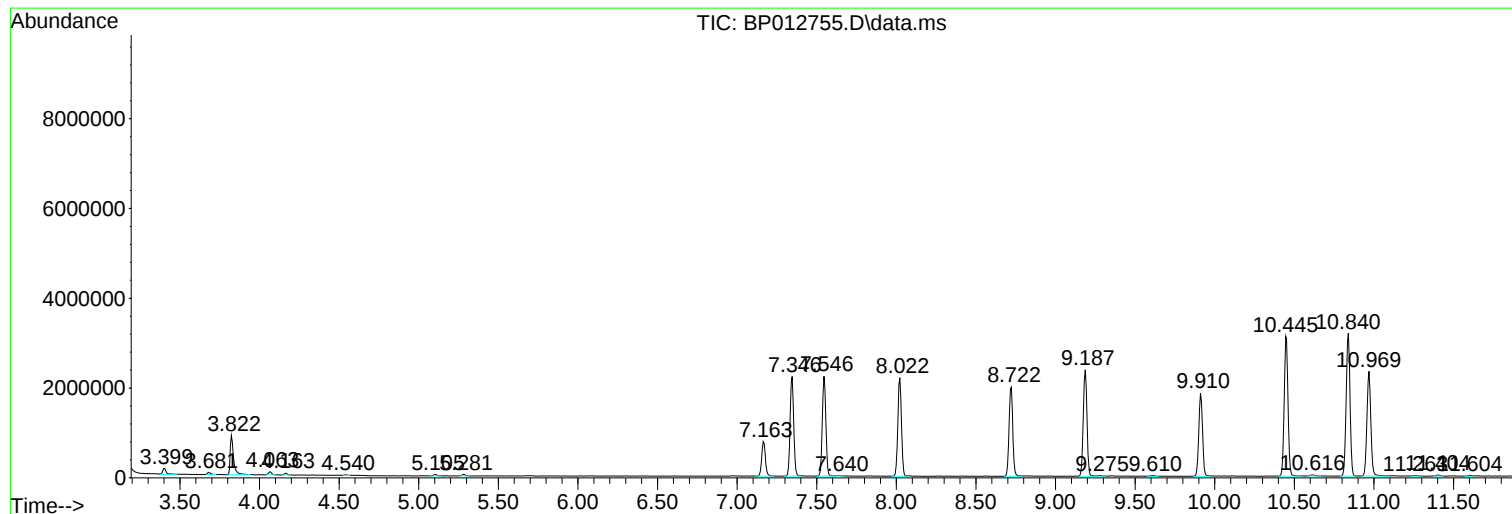

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012755.D
Acq On : 26 Nov 2022 07:55
Operator : CG/JU
Sample : N5603-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012755.D
Acq On : 26 Nov 2022 07:55
Operator : CG/JU
Sample : N5603-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc