

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012757.D
 Acq On : 26 Nov 2022 09:03
 Operator : CG/JU
 Sample : N5651-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1G6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012757.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	26	31	49	rVB2	1244160	2140015	18.78%	1.818%
2	3.822	105	108	126	rBV	802784	1150721	10.10%	0.978%
3	4.064	145	149	155	rVB	66615	99526	0.87%	0.085%
4	4.164	162	166	171	rBV	41539	55652	0.49%	0.047%
5	4.546	227	231	237	rVB5	13978	22024	0.19%	0.019%
6	4.705	251	258	269	rBV	220218	344744	3.03%	0.293%
7	5.105	322	326	330	rBV4	20156	32702	0.29%	0.028%
8	6.969	638	643	648	rBV6	8178	13839	0.12%	0.012%
9	7.163	670	676	687	rVB	565779	912193	8.00%	0.775%
10	7.346	699	707	716	rBV	2075091	3266316	28.66%	2.775%
11	7.546	734	741	752	rBV	1969848	3020699	26.51%	2.566%
12	7.640	754	757	763	rVB3	13954	21120	0.19%	0.018%
13	8.022	813	822	828	rBV	1949454	3064904	26.89%	2.604%
14	8.081	828	832	839	rVB	38692	56735	0.50%	0.048%
15	8.716	933	940	953	rBV	1528473	2476268	21.73%	2.104%
16	9.187	1012	1020	1029	rBV	2169001	3453795	30.31%	2.934%
17	9.275	1031	1035	1042	rVV5	16414	31306	0.27%	0.027%
18	9.351	1042	1048	1052	rVV9	9367	14655	0.13%	0.012%
19	9.610	1086	1092	1096	rBV2	31922	52336	0.46%	0.044%
20	9.910	1132	1143	1158	rBV	1600683	2597620	22.79%	2.207%
21	10.446	1226	1234	1246	rBV	2606239	4298485	37.72%	3.652%
22	10.616	1260	1263	1268	rBV7	8573	11728	0.10%	0.010%
23	10.840	1291	1301	1309	rBV	2562715	4325404	37.95%	3.675%
24	10.969	1313	1323	1336	rBV	2231625	3868895	33.95%	3.287%
25	12.416	1564	1569	1577	rVB	50388	84918	0.75%	0.072%
26	13.263	1709	1713	1718	rBV8	7013	13382	0.12%	0.011%
27	13.387	1729	1734	1739	rBV6	7246	13031	0.11%	0.011%
28	13.481	1747	1750	1755	rVB4	11610	14471	0.13%	0.012%
29	13.545	1755	1761	1768	rVV4	21581	38036	0.33%	0.032%
30	13.622	1768	1774	1781	rVB5	17937	34482	0.30%	0.029%
31	13.975	1829	1834	1839	rBV5	24012	37299	0.33%	0.032%
32	14.063	1842	1849	1865	rVV	4428131	6284110	55.14%	5.339%
33	14.187	1865	1870	1874	rVB8	13466	23644	0.21%	0.020%
34	14.298	1885	1889	1891	rBV4	19478	28856	0.25%	0.025%
35	14.351	1891	1898	1911	rVB	5435736	8280836	72.66%	7.035%
36	14.551	1929	1932	1936	rVB6	10400	12858	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012757.D
 Acq On : 26 Nov 2022 09:03
 Operator : CG/JU
 Sample : N5651-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1G6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	14.657	1939	1950	1958	rVV	3606626	5279544	46.33%	4.485%
38	14.728	1958	1962	1967	rVB8	8798	16640	0.15%	0.014%
39	14.828	1974	1979	1987	rBV	244082	392332	3.44%	0.333%
40	15.063	2014	2019	2025	rVB7	25409	41990	0.37%	0.036%
41	15.463	2083	2087	2091	rBV5	8358	15635	0.14%	0.013%
42	15.645	2111	2118	2130	rBV	7077986	9981937	87.59%	8.480%
43	15.751	2130	2136	2147	rBV	1250759	1725857	15.14%	1.466%
44	15.886	2155	2159	2166	rVB3	33727	57010	0.50%	0.048%
45	16.439	2245	2253	2258	rVB6	11096	23975	0.21%	0.020%
46	16.675	2285	2293	2296	rBV10	4648	13501	0.12%	0.011%
47	16.792	2307	2313	2317	rBV5	14823	21468	0.19%	0.018%
48	16.945	2335	2339	2342	rVB4	10025	17345	0.15%	0.015%
49	17.198	2379	2382	2388	rVB4	7693	13600	0.12%	0.012%
50	17.410	2411	2418	2428	rBV	3768429	5190451	45.55%	4.410%
51	17.510	2428	2435	2454	rVV	6945503	9689016	85.02%	8.231%
52	18.075	2527	2531	2535	rVB2	34541	43716	0.38%	0.037%
53	18.157	2542	2545	2549	rVB6	11387	16232	0.14%	0.014%
54	18.280	2561	2566	2575	rBV	139039	198377	1.74%	0.169%
55	18.357	2577	2579	2585	rVB2	16444	19026	0.17%	0.016%
56	19.110	2704	2707	2710	rBV5	14341	17184	0.15%	0.015%
57	19.227	2722	2727	2736	rVB	105671	140337	1.23%	0.119%
58	19.316	2737	2742	2748	rBV2	74871	112331	0.99%	0.095%
59	19.380	2748	2753	2760	rBV2	81581	169660	1.49%	0.144%
60	19.457	2762	2766	2771	rVV	321305	359694	3.16%	0.306%
61	19.510	2771	2775	2783	rVB3	68767	95651	0.84%	0.081%
62	19.733	2807	2813	2826	rBV	8155589	10603483	93.04%	9.008%
63	21.186	3057	3060	3064	rBV2	164416	194588	1.71%	0.165%
64	21.492	3107	3112	3123	rBV	3954956	5257526	46.13%	4.467%
65	21.598	3127	3130	3135	rBV2	138964	204146	1.79%	0.173%
66	22.804	3332	3335	3348	rVB2	212415	344420	3.02%	0.293%
67	23.845	3505	3512	3521	rBV2	5713907	11396155	100.00%	9.682%
68	24.010	3533	3540	3553	rVB2	2858472	5856995	51.39%	4.976%




Sum of corrected areas: 117707427

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012757.D
Acq On : 26 Nov 2022 09:03
Operator : CG/JU
Sample : N5651-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1G6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

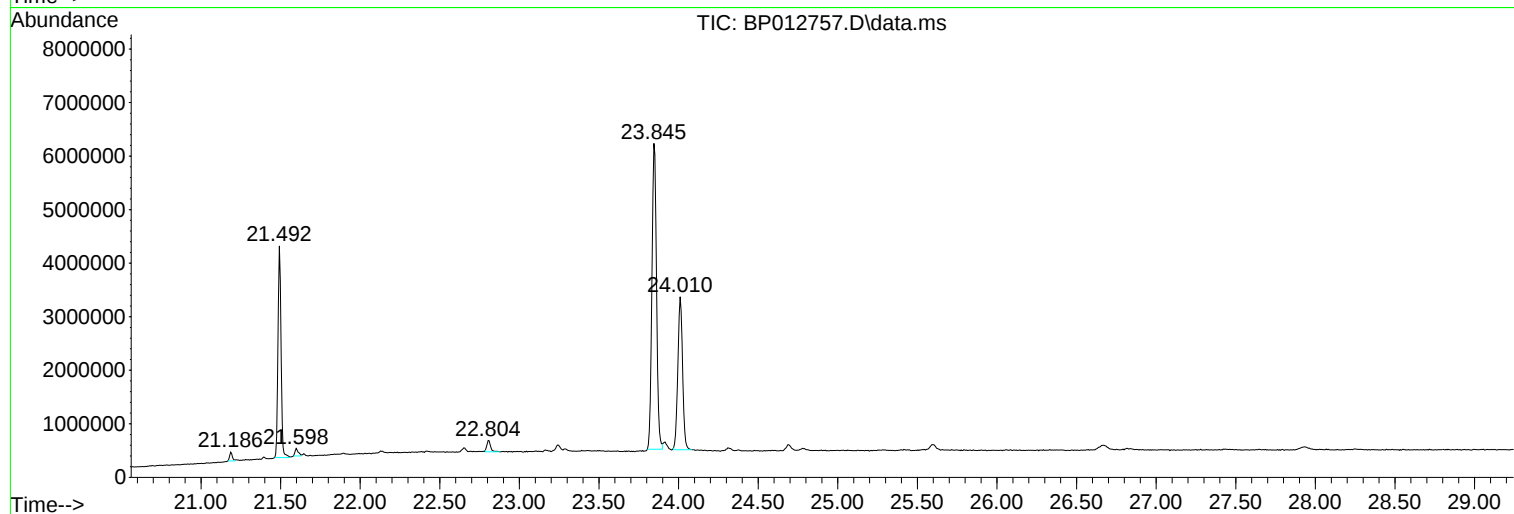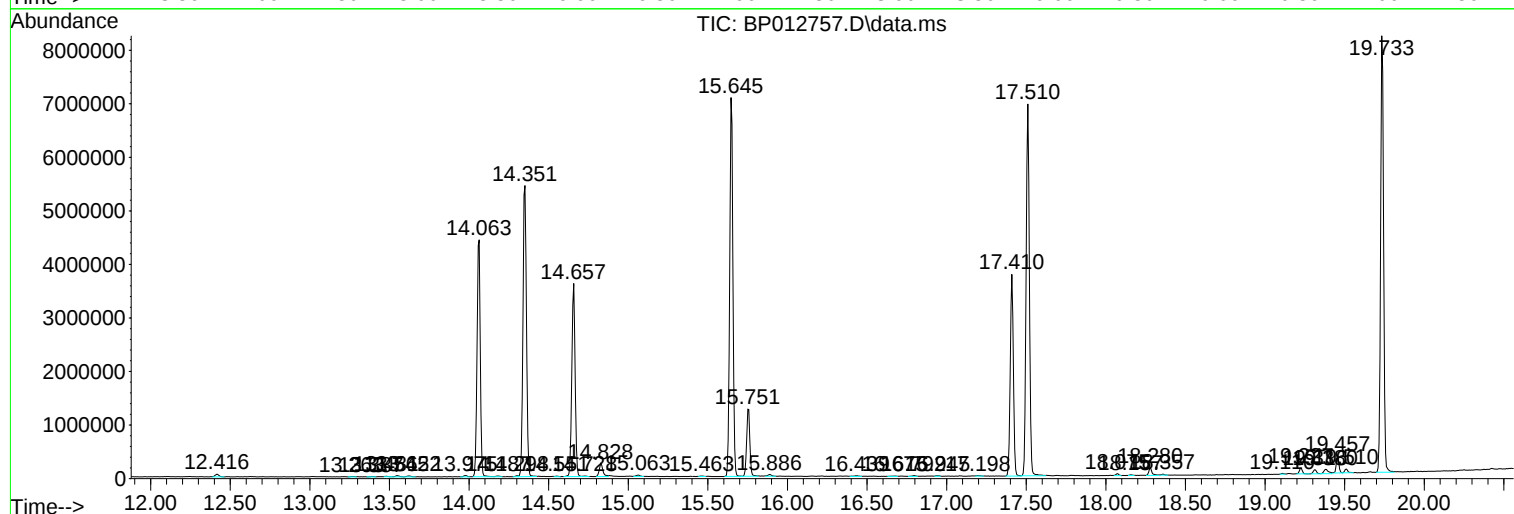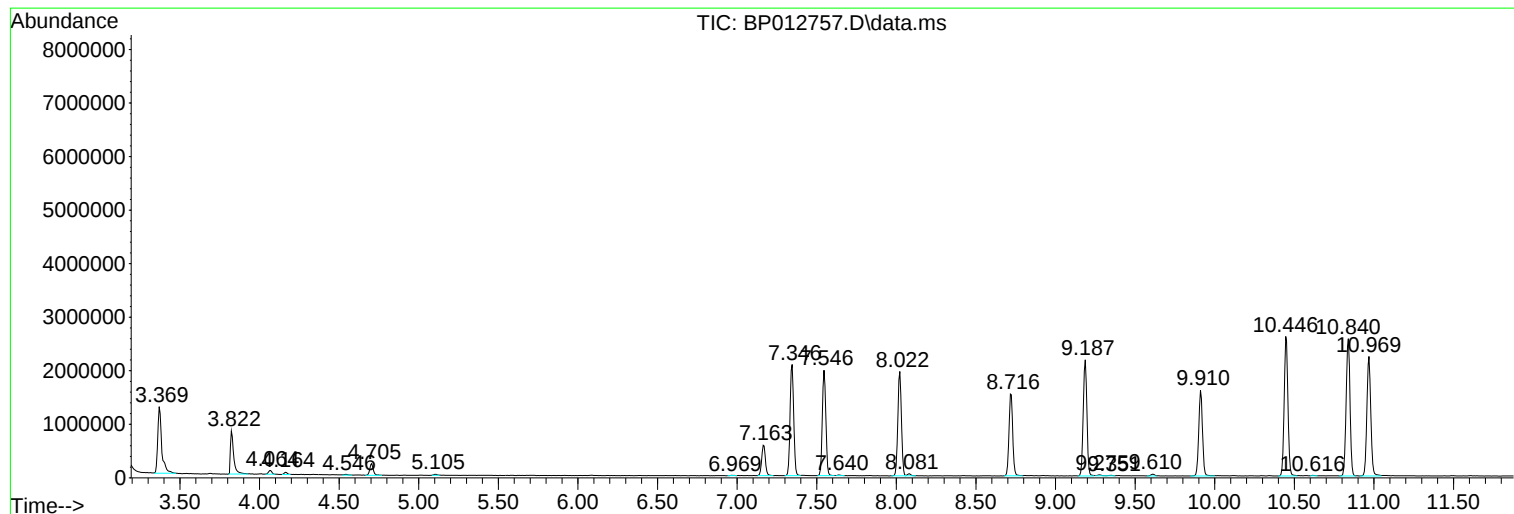

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012757.D
Acq On : 26 Nov 2022 09:03
Operator : CG/JU
Sample : N5651-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1G6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012757.D
Acq On : 26 Nov 2022 09:03
Operator : CG/JU
Sample : N5651-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1G6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
