

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012758.D
 Acq On : 26 Nov 2022 09:37
 Operator : CG/JU
 Sample : N5651-11
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1K3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012758.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	27	31	34	rBV	126384	183740	1.62%	0.155%
2	3.399	34	36	46	rVB	137502	177745	1.57%	0.150%
3	3.687	82	85	92	rVB3	13803	23513	0.21%	0.020%
4	3.823	105	108	120	rBV	689276	982354	8.65%	0.827%
5	4.070	145	150	158	rVB	68073	112324	0.99%	0.095%
6	4.164	162	166	170	rVB	42389	58460	0.51%	0.049%
7	4.705	253	258	263	rBV	59202	91892	0.81%	0.077%
8	5.105	320	326	332	rBV4	23502	37567	0.33%	0.032%
9	6.969	639	643	650	rBV5	10652	21322	0.19%	0.018%
10	7.164	669	676	690	rBV	567334	884277	7.79%	0.744%
11	7.346	699	707	716	rBV	2218134	3473524	30.60%	2.923%
12	7.546	732	741	754	rBV	2007840	3088887	27.21%	2.599%
13	7.640	754	757	763	rVB7	13143	19702	0.17%	0.017%
14	8.022	815	822	828	rBV	2081414	3321066	29.25%	2.794%
15	8.081	828	832	839	rVB	38956	62008	0.55%	0.052%
16	8.716	933	940	952	rBV	1622781	2614834	23.03%	2.200%
17	9.187	1011	1020	1031	rBV	2369988	3779012	33.29%	3.180%
18	9.275	1031	1035	1040	rVB6	17102	29161	0.26%	0.025%
19	9.610	1088	1092	1098	rVB3	25973	38763	0.34%	0.033%
20	9.910	1134	1143	1153	rBV	1761688	2848714	25.09%	2.397%
21	10.116	1173	1178	1184	rVB9	11077	19067	0.17%	0.016%
22	10.446	1226	1234	1248	rBV	2844898	4743800	41.79%	3.991%
23	10.834	1291	1300	1309	rBV	2915920	4924484	43.38%	4.143%
24	10.969	1314	1323	1338	rBV	2430749	4199417	36.99%	3.533%
25	11.610	1427	1432	1437	rBV7	8847	16157	0.14%	0.014%
26	12.104	1512	1516	1521	rVB6	7028	12140	0.11%	0.010%
27	12.416	1562	1569	1576	rBV	53939	93841	0.83%	0.079%
28	12.622	1598	1604	1610	rVB9	7183	16515	0.15%	0.014%
29	13.269	1709	1714	1721	rVB9	7639	16377	0.14%	0.014%
30	13.551	1757	1762	1767	rBV2	33129	53279	0.47%	0.045%
31	13.628	1769	1775	1779	rBV4	12478	19093	0.17%	0.016%
32	13.975	1829	1834	1840	rBV7	12200	24440	0.22%	0.021%
33	14.063	1842	1849	1861	rVV	5180430	7192519	63.36%	6.052%
34	14.181	1865	1869	1874	rVB8	7374	13284	0.12%	0.011%
35	14.298	1885	1889	1891	rBV4	10252	14185	0.12%	0.012%
36	14.351	1891	1898	1906	rVV	6445055	9414198	82.92%	7.921%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012758.D
 Acq On : 26 Nov 2022 09:37
 Operator : CG/JU
 Sample : N5651-11
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH1K3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	14.657	1943	1950	1959	rBV	4256378	6308326	55.57%	5.308%
38	14.828	1972	1979	1987	rBV	235947	384107	3.38%	0.323%
39	15.063	2013	2019	2024	rVB7	33687	54454	0.48%	0.046%
40	15.392	2070	2075	2080	rVB7	7139	11722	0.10%	0.010%
41	15.651	2110	2119	2130	rBV	7577586	11352700	100.00%	9.552%
42	15.751	2130	2136	2148	rVV	1417361	1953697	17.21%	1.644%
43	15.887	2155	2159	2166	rVB2	35518	59457	0.52%	0.050%
44	16.434	2249	2252	2257	rVB5	11744	16406	0.14%	0.014%
45	16.792	2309	2313	2322	rVB10	11583	20934	0.18%	0.018%
46	17.087	2360	2363	2368	rVB7	8815	14161	0.12%	0.012%
47	17.163	2371	2376	2379	rBV7	13367	21782	0.19%	0.018%
48	17.410	2411	2418	2428	rBV	4415913	6093838	53.68%	5.127%
49	17.510	2428	2435	2449	rVV	7785168	10716407	94.40%	9.016%
50	18.075	2527	2531	2535	rBV3	23001	29297	0.26%	0.025%
51	18.281	2561	2566	2576	rBV	158267	228354	2.01%	0.192%
52	18.357	2577	2579	2584	rVB2	15938	18658	0.16%	0.016%
53	19.316	2737	2742	2747	rBV2	79667	119826	1.06%	0.101%
54	19.381	2748	2753	2758	rVV	76423	128697	1.13%	0.108%
55	19.457	2762	2766	2771	rVV	133947	152719	1.35%	0.128%
56	19.510	2771	2775	2783	rVV2	102661	138127	1.22%	0.116%
57	19.657	2798	2800	2803	rBV4	17286	16631	0.15%	0.014%
58	19.733	2807	2813	2825	rBV	7556177	10230712	90.12%	8.608%
59	21.492	3107	3112	3123	rBV	3316399	4498666	39.63%	3.785%
60	23.845	3505	3512	3521	rBV	4306436	8945082	78.79%	7.526%
61	24.010	3533	3540	3550	rVB2	2315861	4717604	41.55%	3.969%




Sum of corrected areas: 118854025

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012758.D
Acq On : 26 Nov 2022 09:37
Operator : CG/JU
Sample : N5651-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1K3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

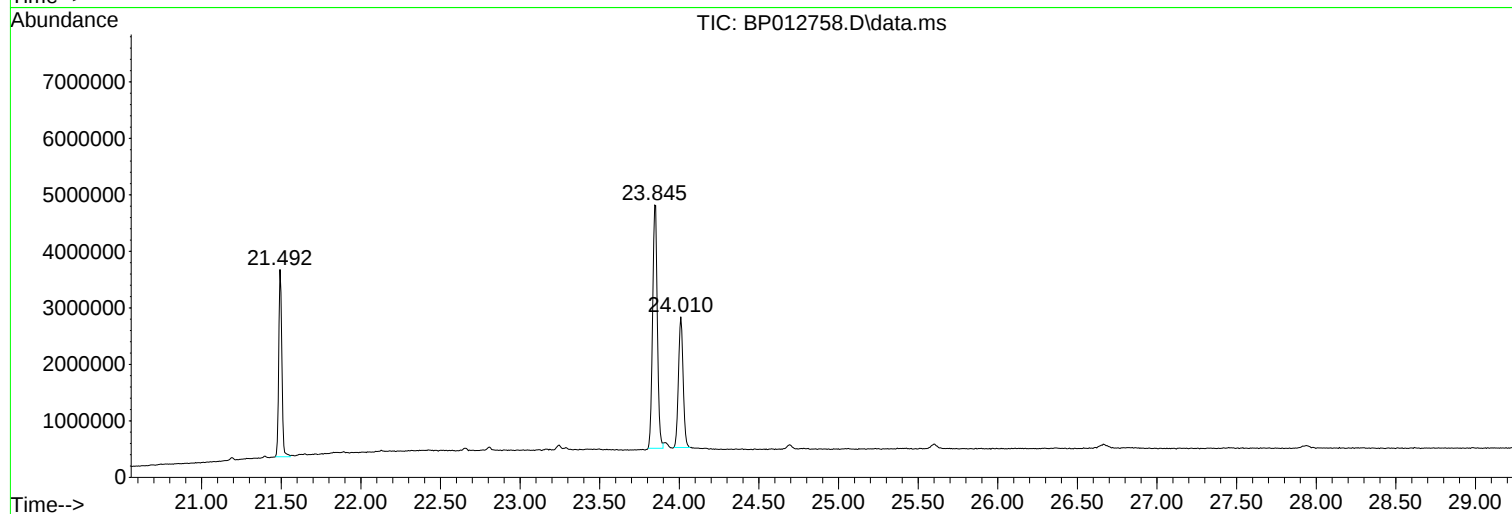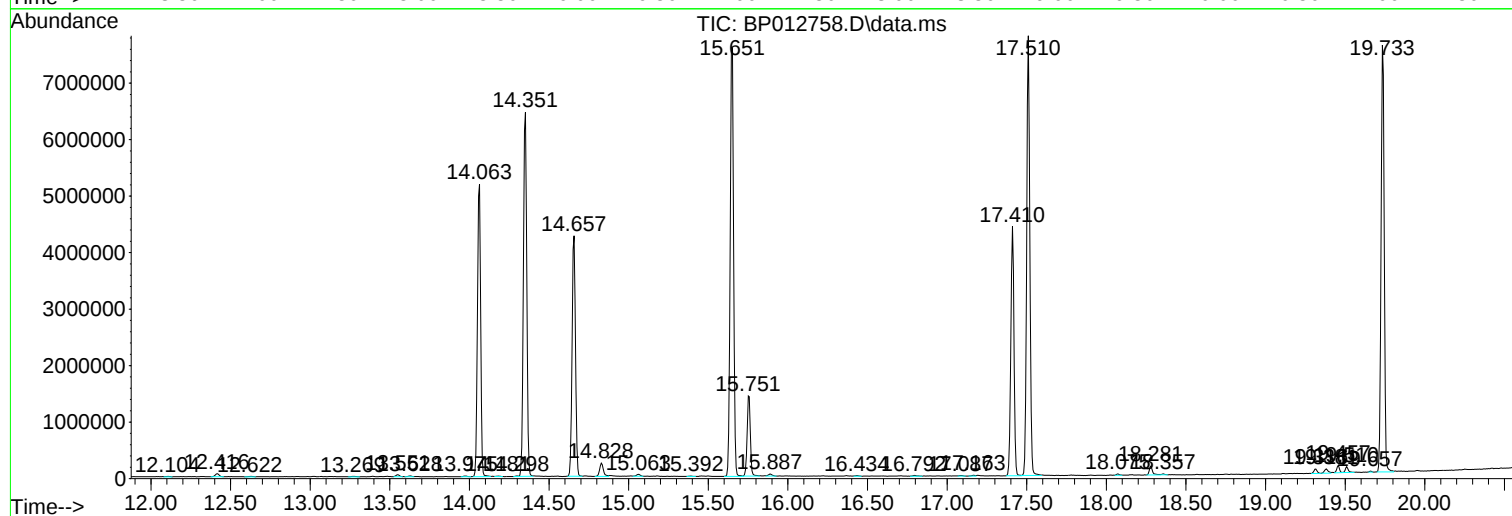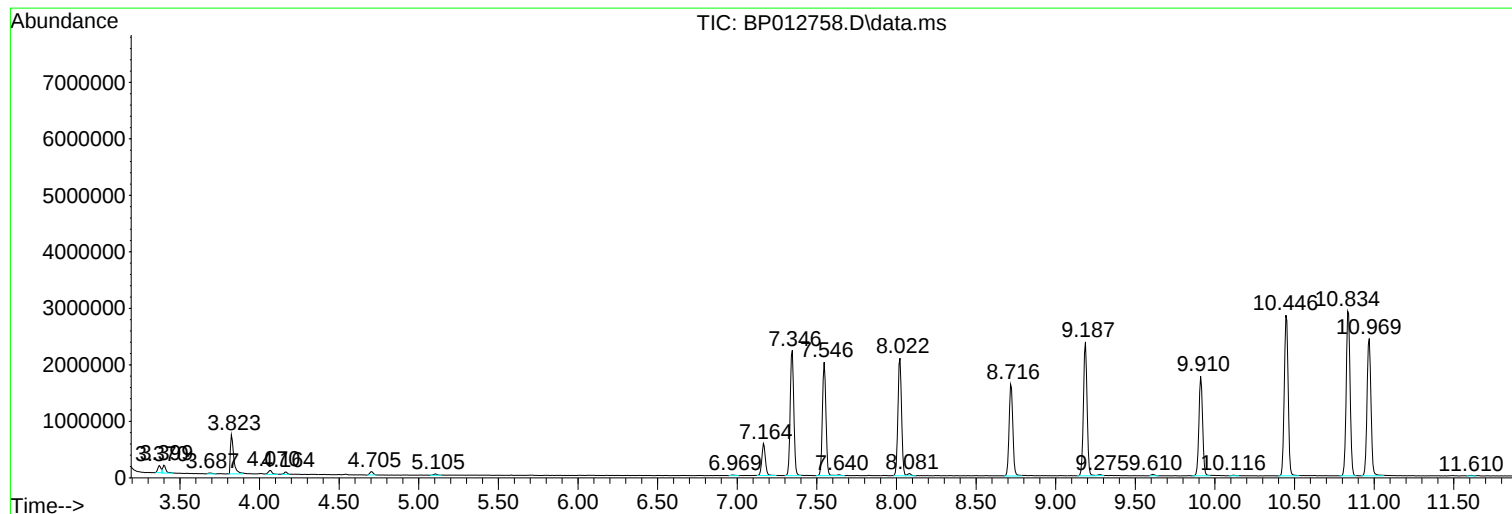

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012758.D
Acq On : 26 Nov 2022 09:37
Operator : CG/JU
Sample : N5651-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1K3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012758.D
Acq On : 26 Nov 2022 09:37
Operator : CG/JU
Sample : N5651-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH1K3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc