

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012761.D
 Acq On : 26 Nov 2022 11:20
 Operator : CG/JU
 Sample : PB149108BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK108

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012761.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	46	rVB	173177	230588	1.63%	0.158%
2	3.822	104	108	133	rBV	1998509	3095140	21.92%	2.125%
3	4.164	162	166	171	rBV	41747	61376	0.43%	0.042%
4	7.163	669	676	689	rBV	2295461	3658154	25.91%	2.512%
5	7.346	700	707	717	rVB	2019347	3158761	22.37%	2.169%
6	7.546	734	741	754	rBV	2361568	3688719	26.12%	2.533%
7	8.022	813	822	830	rBV	2186969	3489903	24.71%	2.396%
8	8.716	932	940	954	rBV	2862811	4707670	33.34%	3.232%
9	9.187	1011	1020	1033	rBV	2205152	3524698	24.96%	2.420%
10	9.910	1134	1143	1155	rBV	1829745	2856717	20.23%	1.961%
11	10.446	1227	1234	1250	rBV	2998840	4903959	34.73%	3.367%
12	10.840	1291	1301	1309	rBV	3156619	5432013	38.47%	3.730%
13	10.969	1315	1323	1334	rBV	2994241	5056586	35.81%	3.472%
14	12.416	1564	1569	1576	rVB2	51186	81218	0.58%	0.056%
15	13.622	1770	1774	1781	rVB4	12353	21531	0.15%	0.015%
16	14.063	1841	1849	1863	rBV	5667797	7799895	55.24%	5.355%
17	14.351	1890	1898	1910	rBV	6507943	9518247	67.40%	6.535%
18	14.657	1942	1950	1958	rBV	5376470	7863482	55.69%	5.399%
19	14.834	1973	1980	1995	rBV	2255652	3227789	22.86%	2.216%
20	15.063	2016	2019	2023	rVB6	13764	20037	0.14%	0.014%
21	15.651	2111	2119	2130	rBV	8092716	11969950	84.77%	8.218%
22	15.757	2130	2137	2151	rVV	2008395	2705644	19.16%	1.858%
23	15.886	2154	2159	2168	rVB2	40029	69772	0.49%	0.048%
24	16.433	2248	2252	2256	rBV6	10886	16641	0.12%	0.011%
25	17.192	2377	2381	2386	rBV4	14050	18785	0.13%	0.013%
26	17.410	2410	2418	2428	rBV	6473658	9218274	65.28%	6.329%
27	17.510	2428	2435	2448	rBV	9006626	12773223	90.45%	8.770%
28	18.280	2563	2566	2573	rVB9	8618	14249	0.10%	0.010%
29	19.310	2737	2741	2747	rBV2	93858	137921	0.98%	0.095%
30	19.380	2749	2753	2758	rVV	88279	117630	0.83%	0.081%
31	19.733	2807	2813	2827	rBV	10312252	14121238	100.00%	9.695%
32	21.492	3107	3112	3124	rBV	5790800	7766886	55.00%	5.333%
33	23.845	3505	3512	3521	rBV2	4327539	8572042	60.70%	5.885%
34	24.010	3533	3540	3552	rVB2	2864829	5749242	40.71%	3.947%

Sum of corrected areas: 145647980




Instrument :
BNA_P
ClientSampleId :
SBLK108

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012761.D
Acq On : 26 Nov 2022 11:20
Operator : CG/JU
Sample : PB149108BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK108

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

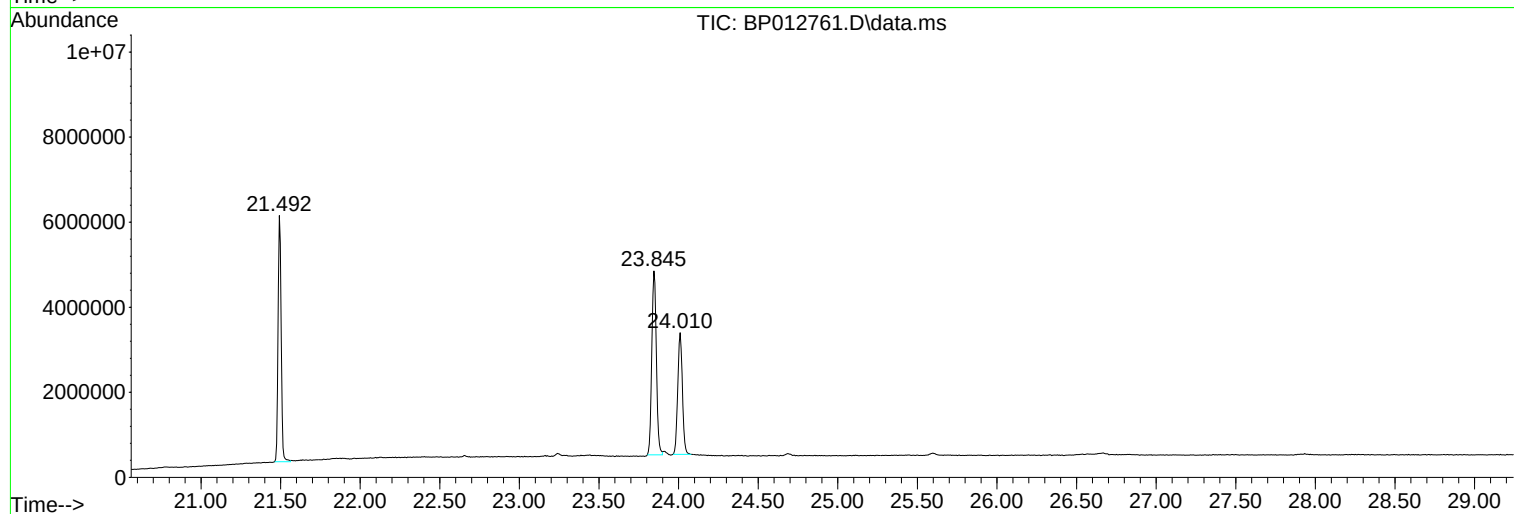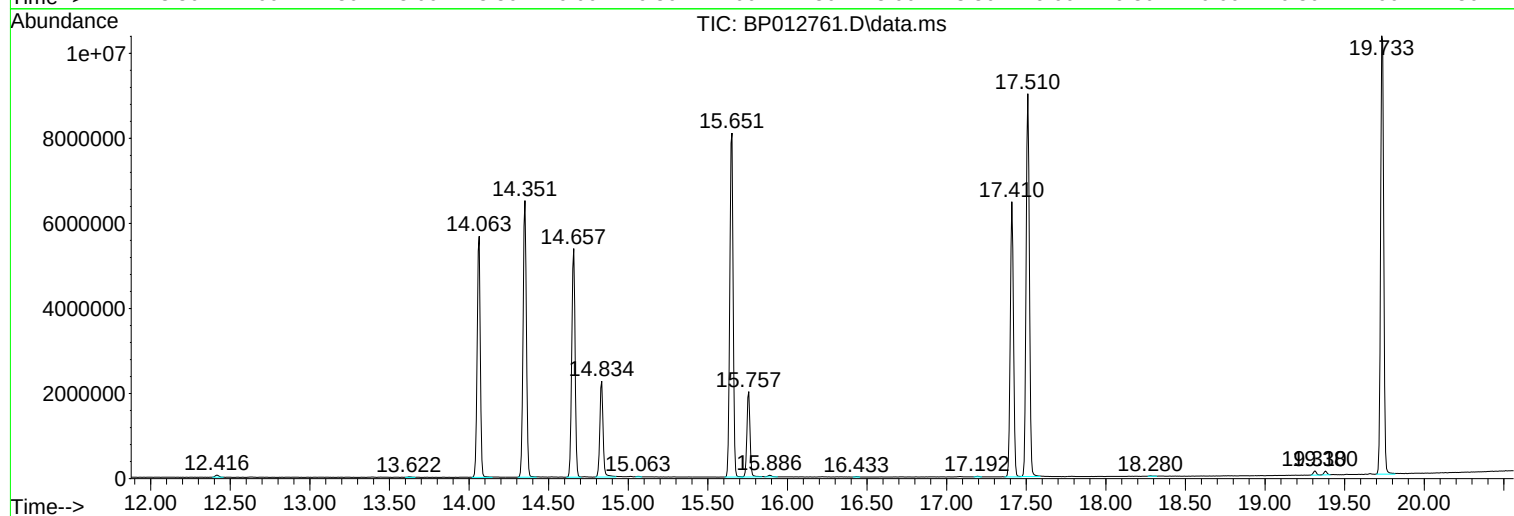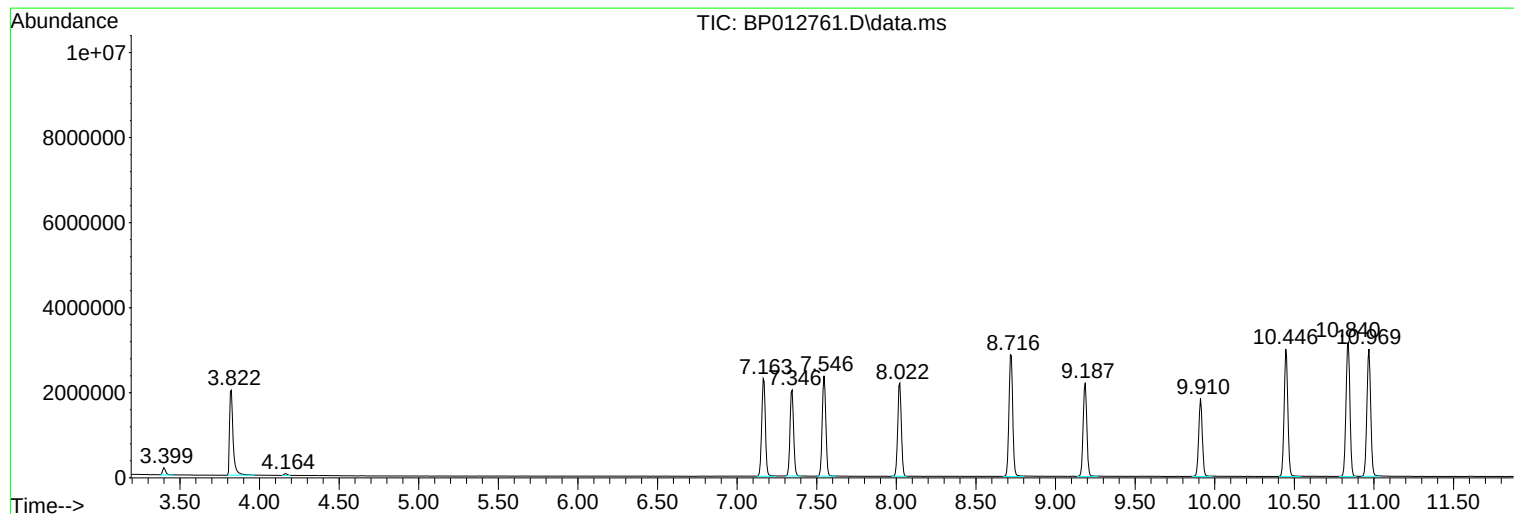

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012761.D
Acq On : 26 Nov 2022 11:20
Operator : CG/JU
Sample : PB149108BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK108

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012761.D
Acq On : 26 Nov 2022 11:20
Operator : CG/JU
Sample : PB149108BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK108

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc