

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012765.D
 Acq On : 26 Nov 2022 13:36
 Operator : CG/JU
 Sample : N5592-05DL 10X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AB0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012765.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	25	31	38	rBV	530472	825132	10.07%	1.536%
2	3.434	38	42	53	rVB	329000	438398	5.35%	0.816%
3	3.840	108	111	118	rBV	41220	67781	0.83%	0.126%
4	4.164	162	166	171	rBV	33686	48631	0.59%	0.091%
5	4.381	201	203	209	rVB7	7981	10196	0.12%	0.019%
6	4.705	251	258	271	rVB	5279778	8193865	100.00%	15.252%
7	5.099	320	325	333	rBV	174898	245865	3.00%	0.458%
8	7.163	671	676	687	rVB	45447	82188	1.00%	0.153%
9	7.340	700	706	713	rBV	157409	251150	3.07%	0.467%
10	7.546	734	741	748	rBV	133431	212401	2.59%	0.395%
11	8.022	814	822	832	rBV	1820478	2882612	35.18%	5.366%
12	8.722	933	941	949	rBV	104811	186549	2.28%	0.347%
13	9.181	1012	1019	1028	rBV	121761	210705	2.57%	0.392%
14	9.605	1087	1091	1098	rVB10	4776	11411	0.14%	0.021%
15	9.910	1137	1143	1154	rVB2	81936	143976	1.76%	0.268%
16	10.446	1225	1234	1246	rBV	179299	335323	4.09%	0.624%
17	10.834	1291	1300	1309	rBV	2595808	4441836	54.21%	8.268%
18	10.969	1315	1323	1333	rBV2	110107	208332	2.54%	0.388%
19	11.610	1427	1432	1438	rBV8	4556	10446	0.13%	0.019%
20	12.351	1549	1558	1566	rBV	69636	121198	1.48%	0.226%
21	13.393	1730	1735	1742	rVB8	5325	11599	0.14%	0.022%
22	14.057	1841	1848	1856	rBV	537505	762468	9.31%	1.419%
23	14.351	1887	1898	1905	rBV	472431	742995	9.07%	1.383%
24	14.657	1942	1950	1964	rBV	4491959	6666423	81.36%	12.409%
25	14.834	1975	1980	1986	rBV7	11602	23634	0.29%	0.044%
26	15.645	2112	2118	2127	rBV	844249	1176382	14.36%	2.190%
27	15.751	2131	2136	2143	rVB2	105743	150861	1.84%	0.281%
28	15.892	2157	2160	2165	rVB7	5495	8238	0.10%	0.015%
29	17.198	2378	2382	2384	rVB3	9600	12062	0.15%	0.022%
30	17.410	2411	2418	2429	rBV	5742461	8062223	98.39%	15.007%
31	17.510	2429	2435	2448	rVV	930482	1353340	16.52%	2.519%
32	18.281	2562	2566	2572	rBV5	30688	48893	0.60%	0.091%
33	18.357	2576	2579	2584	rVB7	19592	26067	0.32%	0.049%
34	19.510	2772	2775	2782	rBV7	31182	49326	0.60%	0.092%
35	19.733	2808	2813	2824	rBV	1211578	1600101	19.53%	2.978%
36	21.492	3107	3112	3127	rBV	5552121	7587196	92.60%	14.123%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012765.D
Acq On : 26 Nov 2022 13:36
Operator : CG/JU
Sample : N5592-05DL 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AB0DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION

37	23.845	3507	3512	3519	rVB	412541	760976	9.29%	1.416%
38	24.010	3533	3540	3552	rVB2	2849123	5752804	70.21%	10.708%




Sum of corrected areas: 53723583

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012765.D
Acq On : 26 Nov 2022 13:36
Operator : CG/JU
Sample : N5592-05DL 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AB0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

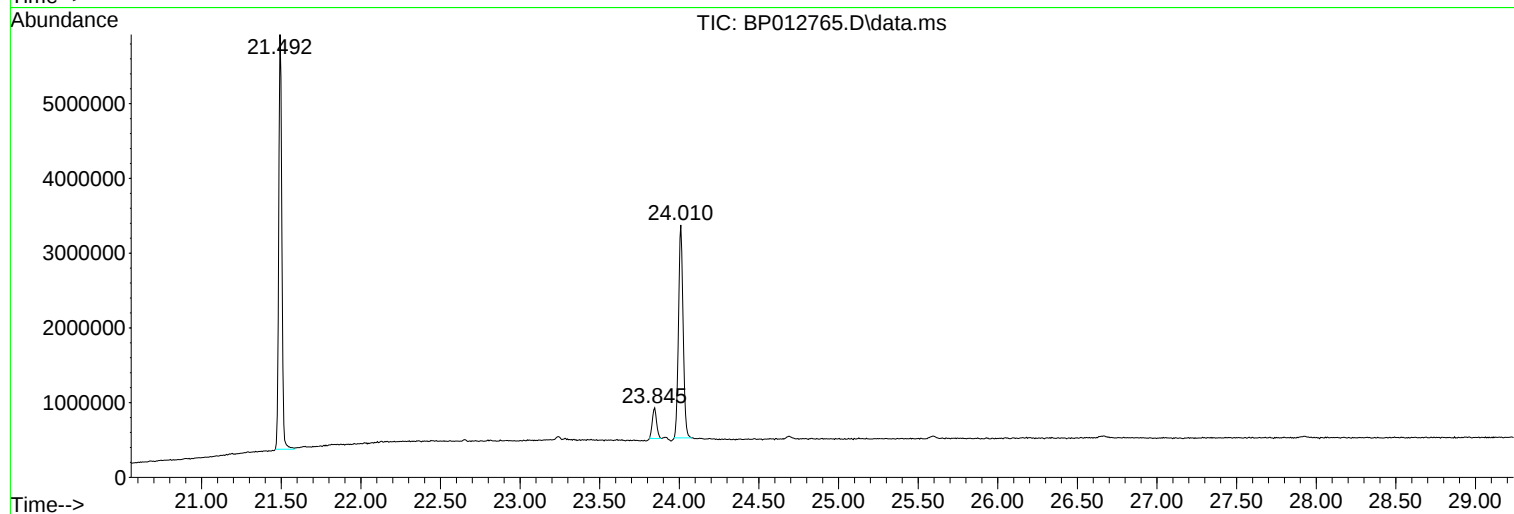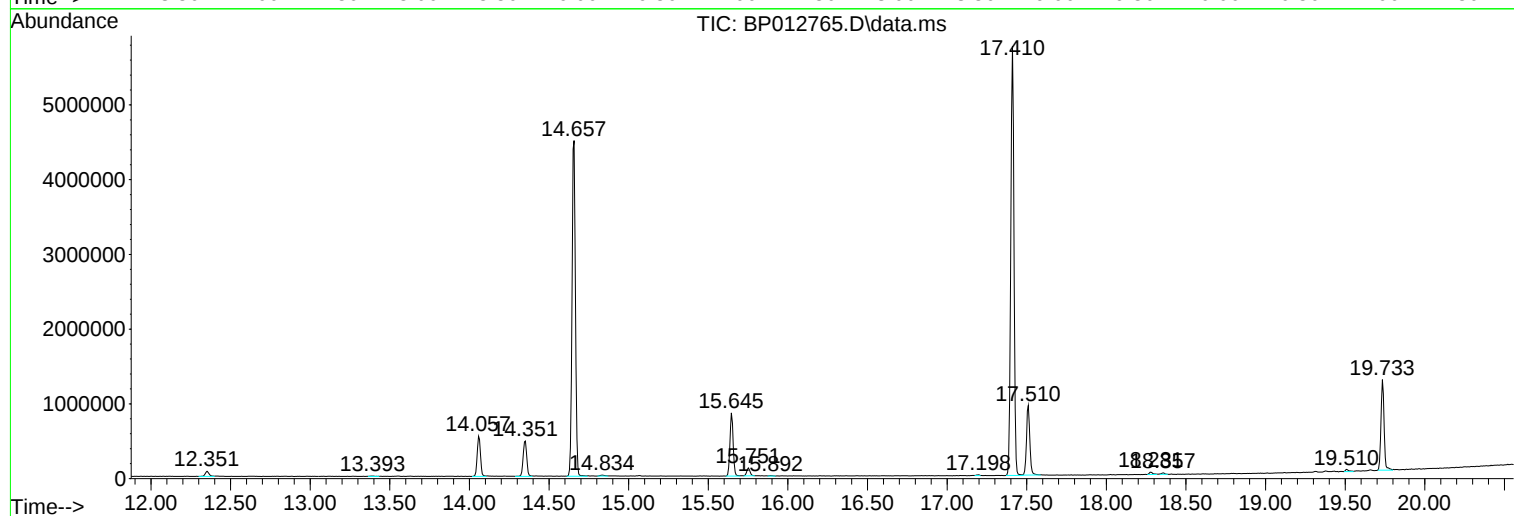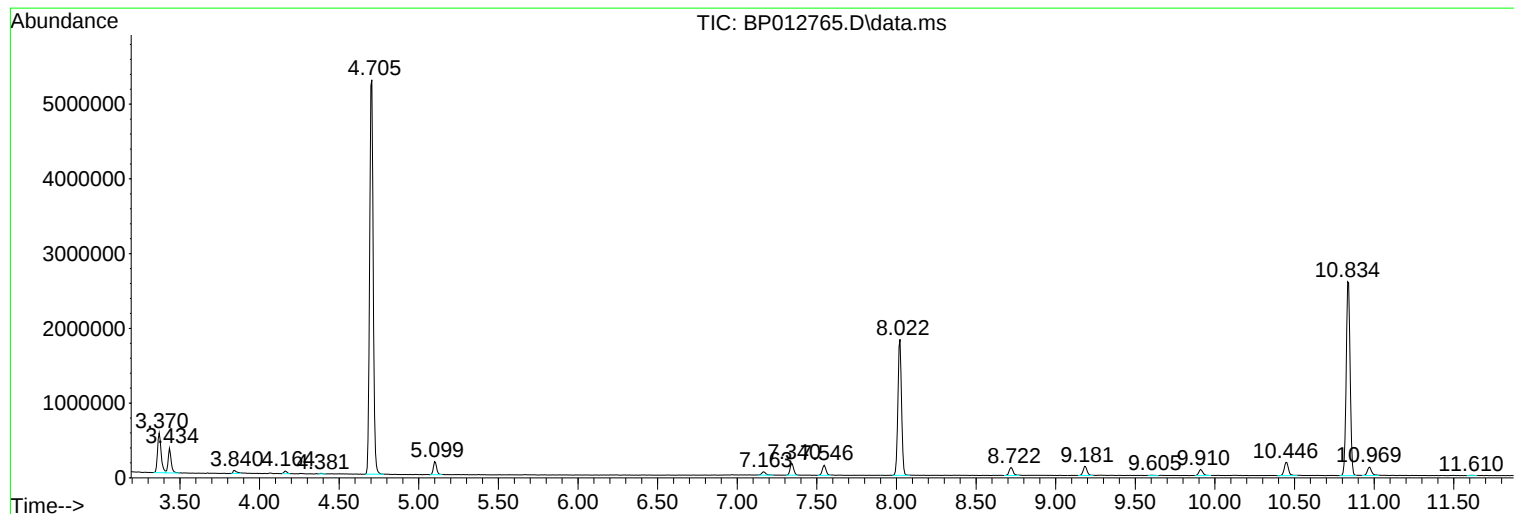

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012765.D
Acq On : 26 Nov 2022 13:36
Operator : CG/JU
Sample : N5592-05DL 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AB0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012765.D
Acq On : 26 Nov 2022 13:36
Operator : CG/JU
Sample : N5592-05DL 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AB0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc