

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012767.D
 Acq On : 26 Nov 2022 14:44
 Operator : CG/JU
 Sample : N5602-08
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012767.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	43	rBV	109423	143619	0.94%	0.112%
2	3.681	81	84	94	rBV	24524	46295	0.30%	0.036%
3	3.822	105	108	124	rBV	666428	996456	6.54%	0.776%
4	4.064	144	149	154	rVB2	54471	84832	0.56%	0.066%
5	4.164	162	166	174	rVB	36921	55128	0.36%	0.043%
6	5.105	320	326	330	rBV3	17209	28279	0.19%	0.022%
7	7.163	669	676	686	rBV	520814	831834	5.46%	0.648%
8	7.346	700	707	717	rVB	1840490	2917115	19.14%	2.272%
9	7.546	734	741	750	rBV	1740264	2697086	17.70%	2.100%
10	7.640	754	757	763	rVB8	13251	19566	0.13%	0.015%
11	8.022	814	822	829	rBV	1759509	2824932	18.54%	2.200%
12	8.716	933	940	952	rBV	1459692	2384261	15.65%	1.857%
13	9.187	1011	1020	1031	rBV	2036378	3243330	21.28%	2.526%
14	9.275	1032	1035	1040	rVB5	10547	17655	0.12%	0.014%
15	9.610	1086	1092	1096	rBV5	11256	18197	0.12%	0.014%
16	9.910	1134	1143	1153	rBV	1547170	2468976	16.20%	1.923%
17	10.446	1225	1234	1247	rBV	2549407	4191025	27.50%	3.264%
18	10.834	1292	1300	1312	rVB	2598431	4409445	28.93%	3.434%
19	10.969	1314	1323	1337	rBV	2291934	3943044	25.87%	3.071%
20	12.416	1563	1569	1574	rBV	47570	78109	0.51%	0.061%
21	13.546	1757	1761	1767	rBV3	28515	49478	0.32%	0.039%
22	13.628	1770	1775	1782	rVB2	13141	22558	0.15%	0.018%
23	13.975	1828	1834	1839	rBV8	13619	22527	0.15%	0.018%
24	14.057	1842	1848	1860	rVV	5408327	7834034	51.41%	6.101%
25	14.298	1884	1889	1891	rBV5	11061	18655	0.12%	0.015%
26	14.351	1891	1898	1906	rVV	6155808	9162495	60.12%	7.136%
27	14.657	1942	1950	1959	rVV	4289372	6325327	41.51%	4.926%
28	14.828	1973	1979	1997	rBV	386296	646913	4.24%	0.504%
29	15.063	2014	2019	2024	rVB5	38110	55953	0.37%	0.044%
30	15.392	2069	2075	2080	rBV2	13273	22559	0.15%	0.018%
31	15.463	2081	2087	2089	rBV3	9627	16119	0.11%	0.013%
32	15.645	2110	2118	2130	rBV	8426688	12345192	81.01%	9.614%
33	15.751	2130	2136	2151	rVV	1838852	2563447	16.82%	1.996%
34	15.887	2155	2159	2166	rVB	36428	60404	0.40%	0.047%
35	16.439	2247	2253	2257	rVB9	10365	17731	0.12%	0.014%
36	17.087	2357	2363	2366	rBV5	11502	21656	0.14%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012767.D
 Acq On : 26 Nov 2022 14:44
 Operator : CG/JU
 Sample : N5602-08
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG0

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	17.410	2411	2418	2426	rBV	5388630	7443640	48.84%	5.797%
38	17.510	2428	2435	2446	rVV	9693536	13636088	89.48%	10.619%
39	17.592	2446	2449	2455	rVB3	38847	56506	0.37%	0.044%
40	18.275	2561	2565	2573	rBV2	77612	118617	0.78%	0.092%
41	19.316	2737	2742	2746	rBV2	106564	152629	1.00%	0.119%
42	19.381	2749	2753	2759	rVV	98237	139998	0.92%	0.109%
43	19.510	2771	2775	2779	rBV4	55365	71082	0.47%	0.055%
44	19.657	2798	2800	2805	rVB6	22594	25241	0.17%	0.020%
45	19.739	2807	2814	2827	rVV	11211202	15239687	100.00%	11.868%
46	21.492	3107	3112	3128	rBV	4552553	6477690	42.51%	5.045%
47	23.845	3505	3512	3531	rBV	4751443	9576989	62.84%	7.458%
48	24.010	3533	3540	3557	rVB2	2290380	4884311	32.05%	3.804%




Sum of corrected areas: 128406710

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012767.D
Acq On : 26 Nov 2022 14:44
Operator : CG/JU
Sample : N5602-08
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

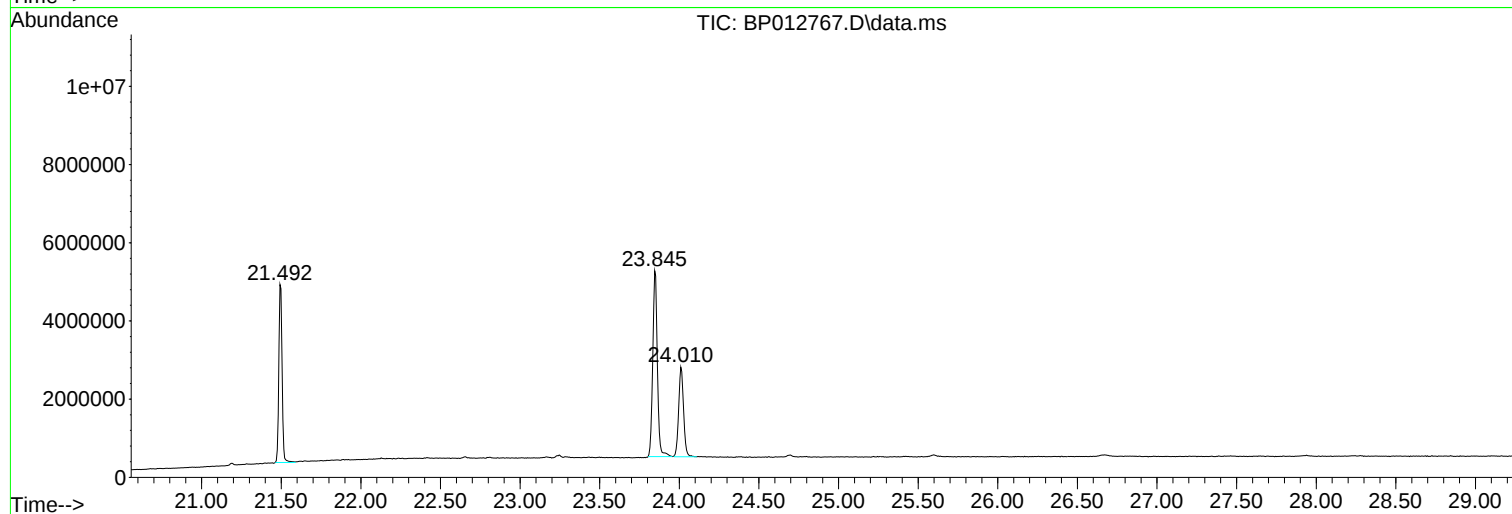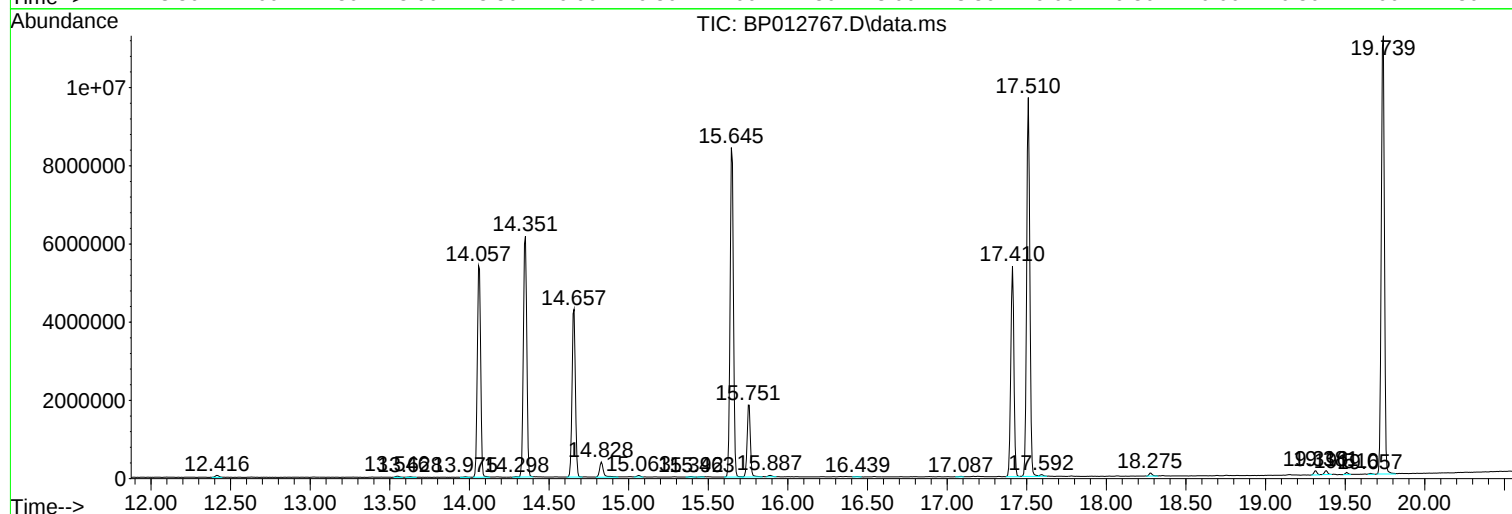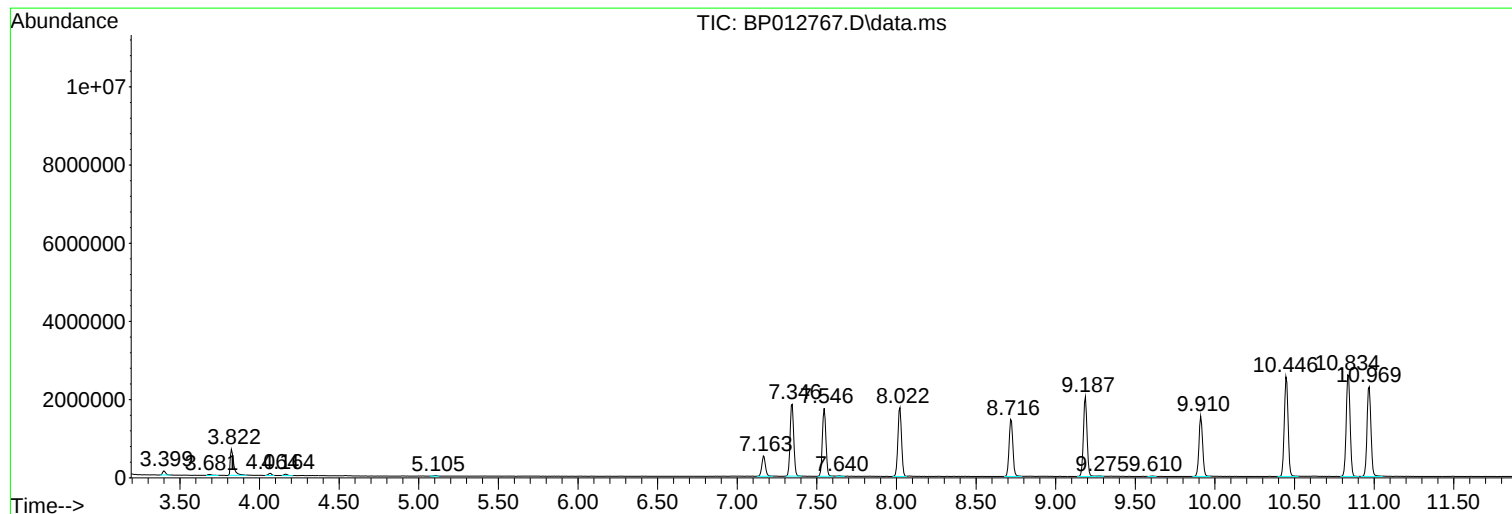

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012767.D
Acq On : 26 Nov 2022 14:44
Operator : CG/JU
Sample : N5602-08
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012767.D
Acq On : 26 Nov 2022 14:44
Operator : CG/JU
Sample : N5602-08
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
