

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012768.D
 Acq On : 26 Nov 2022 15:19
 Operator : CG/JU
 Sample : N5602-09
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012768.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	48	rVB	119873	174248	1.14%	0.133%
2	3.681	80	84	92	rBV	34806	64215	0.42%	0.049%
3	3.822	105	108	126	rBV	549960	831174	5.46%	0.635%
4	4.063	144	149	161	rVB	63253	108422	0.71%	0.083%
5	4.163	161	166	170	rBV	38252	55389	0.36%	0.042%
6	5.105	321	326	331	rBV2	19164	28119	0.18%	0.021%
7	7.163	670	676	692	rVB	606714	951437	6.25%	0.727%
8	7.346	700	707	718	rBV	1897546	3015918	19.81%	2.303%
9	7.546	734	741	751	rBV	1871173	2874297	18.88%	2.195%
10	7.640	754	757	764	rVB6	13954	23272	0.15%	0.018%
11	8.022	811	822	829	rBV	1813418	2883662	18.94%	2.202%
12	8.081	829	832	837	rVB	23135	32325	0.21%	0.025%
13	8.716	933	940	955	rBV	1585078	2558006	16.80%	1.954%
14	9.187	1012	1020	1030	rBV	2047698	3290790	21.61%	2.513%
15	9.281	1031	1036	1043	rVV2	48819	85485	0.56%	0.065%
16	9.351	1044	1048	1056	rVB2	11528	21660	0.14%	0.017%
17	9.610	1088	1092	1098	rVB5	17061	29172	0.19%	0.022%
18	9.910	1136	1143	1152	rBV	1628462	2566195	16.85%	1.960%
19	10.445	1227	1234	1246	rBV	2663797	4336757	28.48%	3.312%
20	10.610	1257	1262	1268	rBV2	17357	33125	0.22%	0.025%
21	10.834	1292	1300	1309	rBV	2650716	4499933	29.55%	3.437%
22	10.969	1314	1323	1338	rBV	2105231	3587121	23.56%	2.740%
23	11.604	1424	1431	1435	rBV8	11278	22300	0.15%	0.017%
24	12.410	1564	1568	1575	rVB2	47290	81561	0.54%	0.062%
25	12.622	1600	1604	1611	rVB6	7785	18387	0.12%	0.014%
26	13.269	1709	1714	1720	rVB5	12665	21283	0.14%	0.016%
27	13.622	1770	1774	1782	rVB5	12930	24880	0.16%	0.019%
28	13.975	1830	1834	1837	rBV6	11661	15434	0.10%	0.012%
29	14.063	1841	1849	1855	rBV	5349744	7578518	49.77%	5.788%
30	14.292	1884	1888	1891	rBV4	19644	29429	0.19%	0.022%
31	14.351	1891	1898	1909	rVV	6109472	9150922	60.10%	6.989%
32	14.428	1909	1911	1918	rVB8	9091	16056	0.11%	0.012%
33	14.657	1942	1950	1959	rBV	4351470	6533404	42.91%	4.990%
34	14.828	1971	1979	1993	rBV	449227	707034	4.64%	0.540%
35	15.063	2014	2019	2026	rVB3	54430	82746	0.54%	0.063%
36	15.392	2068	2075	2080	rBV	23124	33148	0.22%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012768.D
 Acq On : 26 Nov 2022 15:19
 Operator : CG/JU
 Sample : N5602-09
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	15.651	2111	2119	2130	rBV	8084951	12017719	78.93%	9.178%
38	15.757	2130	2137	2148	rVV	1919672	2587392	16.99%	1.976%
39	15.886	2155	2159	2167	rVB6	38339	63357	0.42%	0.048%
40	16.333	2231	2235	2237	rVV4	13362	20368	0.13%	0.016%
41	16.369	2238	2241	2248	rVV9	14794	27933	0.18%	0.021%
42	16.433	2248	2252	2257	rVB7	12603	21708	0.14%	0.017%
43	16.551	2265	2272	2276	rVB5	11851	20557	0.14%	0.016%
44	16.880	2322	2328	2335	rVB5	8148	17258	0.11%	0.013%
45	17.163	2372	2376	2379	rBV2	15001	17612	0.12%	0.013%
46	17.410	2411	2418	2427	rBV	5484036	7748082	50.88%	5.917%
47	17.510	2428	2435	2446	rVV2	9389535	13250744	87.02%	10.120%
48	17.592	2446	2449	2455	rVB6	26000	44050	0.29%	0.034%
49	18.069	2527	2530	2534	rVB5	18113	24515	0.16%	0.019%
50	18.280	2561	2566	2573	rBV	172935	235314	1.55%	0.180%
51	18.351	2575	2578	2586	rVB4	15861	30129	0.20%	0.023%
52	18.698	2634	2637	2642	rVB6	18025	21222	0.14%	0.016%
53	19.151	2711	2714	2718	rBV6	15706	24289	0.16%	0.019%
54	19.316	2737	2742	2746	rBV2	115389	159153	1.05%	0.122%
55	19.380	2748	2753	2759	rVV	107930	161350	1.06%	0.123%
56	19.510	2771	2775	2784	rBV3	121170	159320	1.05%	0.122%
57	19.663	2797	2801	2807	rBV7	28860	48842	0.32%	0.037%
58	19.739	2808	2814	2823	rBV	11360340	15226676	100.00%	11.629%
59	21.192	3058	3061	3065	rBV4	67512	84178	0.55%	0.064%
60	21.498	3107	3113	3120	rBV	5269592	6997004	45.95%	5.344%
61	23.851	3505	3513	3522	rBV2	5024727	10070509	66.14%	7.691%
62	24.015	3534	3541	3557	rVB2	2614041	5495341	36.09%	4.197%




Sum of corrected areas: 130940446

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012768.D
Acq On : 26 Nov 2022 15:19
Operator : CG/JU
Sample : N5602-09
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

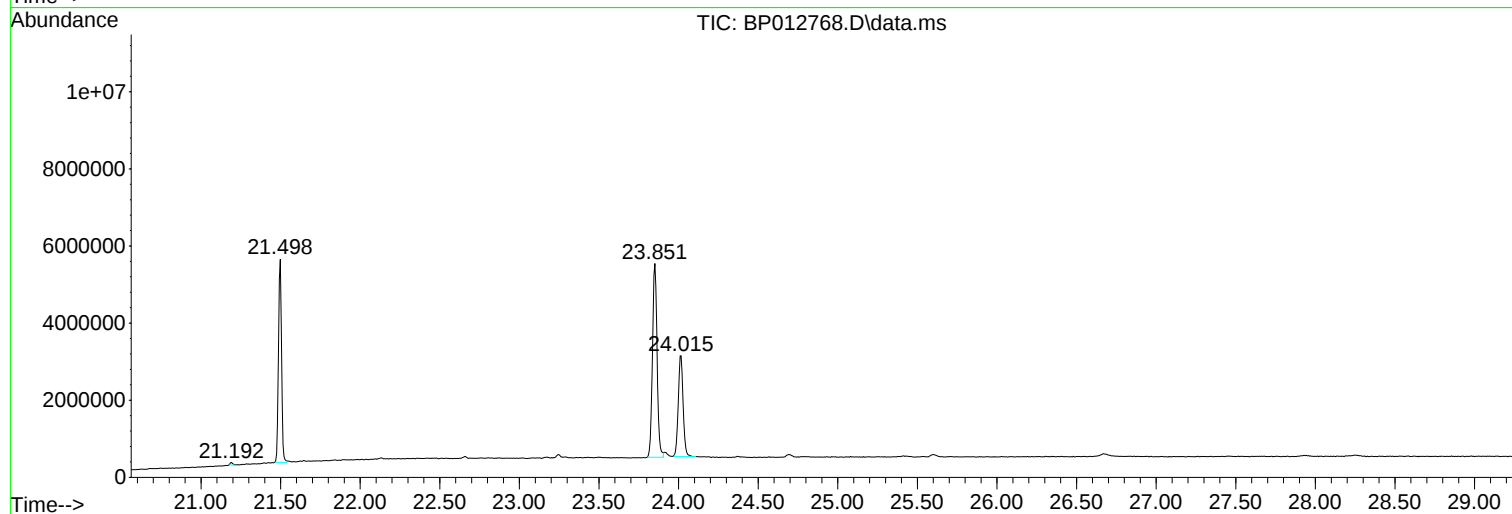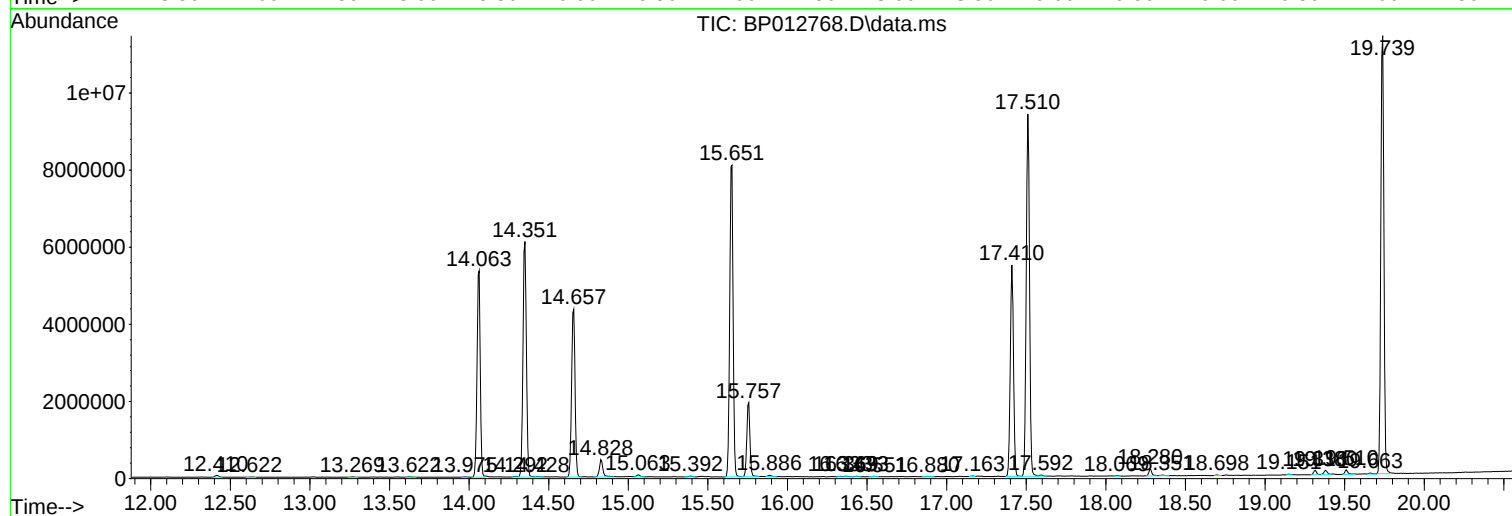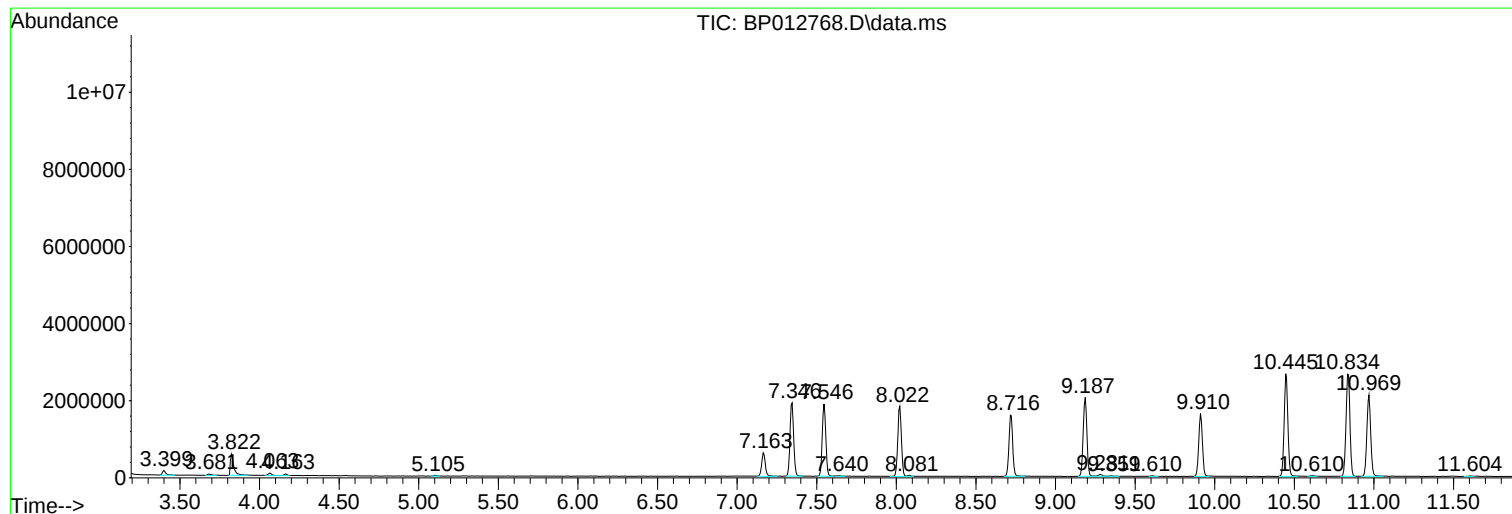

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012768.D
Acq On : 26 Nov 2022 15:19
Operator : CG/JU
Sample : N5602-09
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012768.D
Acq On : 26 Nov 2022 15:19
Operator : CG/JU
Sample : N5602-09
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc