

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012770.D
 Acq On : 26 Nov 2022 16:27
 Operator : CG/JU
 Sample : N5602-11
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012770.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	45	rVB	135799	184007	1.23%	0.133%
2	3.675	80	83	92	rBV	57656	89938	0.60%	0.065%
3	3.822	106	108	119	rBV	645601	941291	6.28%	0.681%
4	4.005	136	139	143	rVV3	13335	17531	0.12%	0.013%
5	4.064	144	149	159	rVB2	70794	118928	0.79%	0.086%
6	4.164	162	166	172	rVB	40368	59116	0.39%	0.043%
7	5.105	321	326	331	rBV2	25041	41274	0.28%	0.030%
8	6.981	638	645	649	rBV6	9966	24588	0.16%	0.018%
9	7.163	669	676	687	rVB	715635	1126870	7.52%	0.815%
10	7.340	698	706	715	rBV	2107447	3362257	22.45%	2.431%
11	7.546	733	741	750	rBV	2164579	3316260	22.14%	2.398%
12	7.640	754	757	767	rVB9	13145	24005	0.16%	0.017%
13	8.022	815	822	829	rBV	2049038	3260435	21.77%	2.358%
14	8.716	933	940	953	rBV	1994076	3176851	21.21%	2.297%
15	9.187	1011	1020	1029	rBV	2298638	3729927	24.90%	2.697%
16	9.287	1031	1037	1045	rVB	90537	148178	0.99%	0.107%
17	9.610	1087	1092	1100	rVB2	23004	38646	0.26%	0.028%
18	9.910	1136	1143	1155	rBV	1833604	2947620	19.68%	2.132%
19	10.116	1173	1178	1185	rBV4	20274	32972	0.22%	0.024%
20	10.446	1225	1234	1249	rBV	3280092	5360744	35.79%	3.877%
21	10.834	1293	1300	1309	rBV	2984643	5106293	34.09%	3.693%
22	10.969	1315	1323	1337	rBV	2130482	3708759	24.76%	2.682%
23	11.604	1425	1431	1435	rBV7	16625	31344	0.21%	0.023%
24	12.416	1562	1569	1575	rVB	56421	90552	0.60%	0.065%
25	12.551	1585	1592	1596	rBV8	10876	24680	0.16%	0.018%
26	12.810	1631	1636	1643	rBV7	12275	23838	0.16%	0.017%
27	13.263	1709	1713	1718	rVB8	9249	16080	0.11%	0.012%
28	13.628	1772	1775	1782	rVB4	13896	24162	0.16%	0.017%
29	14.063	1840	1849	1859	rBV	6021942	8700301	58.08%	6.292%
30	14.351	1891	1898	1905	rVB	7056857	10428924	69.62%	7.542%
31	14.551	1929	1932	1939	rVB4	18259	32841	0.22%	0.024%
32	14.657	1942	1950	1958	rVV	4942939	7208521	48.12%	5.213%
33	14.722	1959	1961	1965	rVB4	12753	17806	0.12%	0.013%
34	14.828	1972	1979	1987	rBV	521046	834390	5.57%	0.603%
35	14.992	2003	2007	2013	rBV7	19223	37010	0.25%	0.027%
36	15.057	2014	2018	2024	rVV8	30017	49724	0.33%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012770.D
 Acq On : 26 Nov 2022 16:27
 Operator : CG/JU
 Sample : N5602-11
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	15.645	2112	2118	2131	rBV	9304277	13375309	89.29%	9.673%
38	15.757	2131	2137	2145	rBV	2268705	3102712	20.71%	2.244%
39	15.886	2156	2159	2165	rVB2	44581	64456	0.43%	0.047%
40	16.792	2311	2313	2318	rVB6	20428	21946	0.15%	0.016%
41	17.410	2412	2418	2428	rBV	5740124	8154629	54.44%	5.897%
42	17.510	2428	2435	2444	rBV2	9768207	13903436	92.82%	10.055%
43	18.075	2528	2531	2535	rVB	52035	61973	0.41%	0.045%
44	18.280	2562	2566	2572	rBV	276494	385861	2.58%	0.279%
45	19.316	2738	2742	2748	rBV	126790	166040	1.11%	0.120%
46	19.380	2749	2753	2758	rVV	128885	217902	1.45%	0.158%
47	19.510	2772	2775	2784	rBV	166411	226695	1.51%	0.164%
48	19.739	2808	2814	2825	rVB	10822067	14979452	100.00%	10.833%
49	21.192	3058	3061	3065	rVB2	126933	153679	1.03%	0.111%
50	21.498	3107	3113	3124	rBV	4379789	6074000	40.55%	4.393%
51	23.851	3505	3513	3521	rBV	4174959	8453945	56.44%	6.114%
52	24.010	3534	3540	3552	rVB2	2203648	4600875	30.71%	3.327%




Sum of corrected areas: 138279573

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012770.D
Acq On : 26 Nov 2022 16:27
Operator : CG/JU
Sample : N5602-11
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

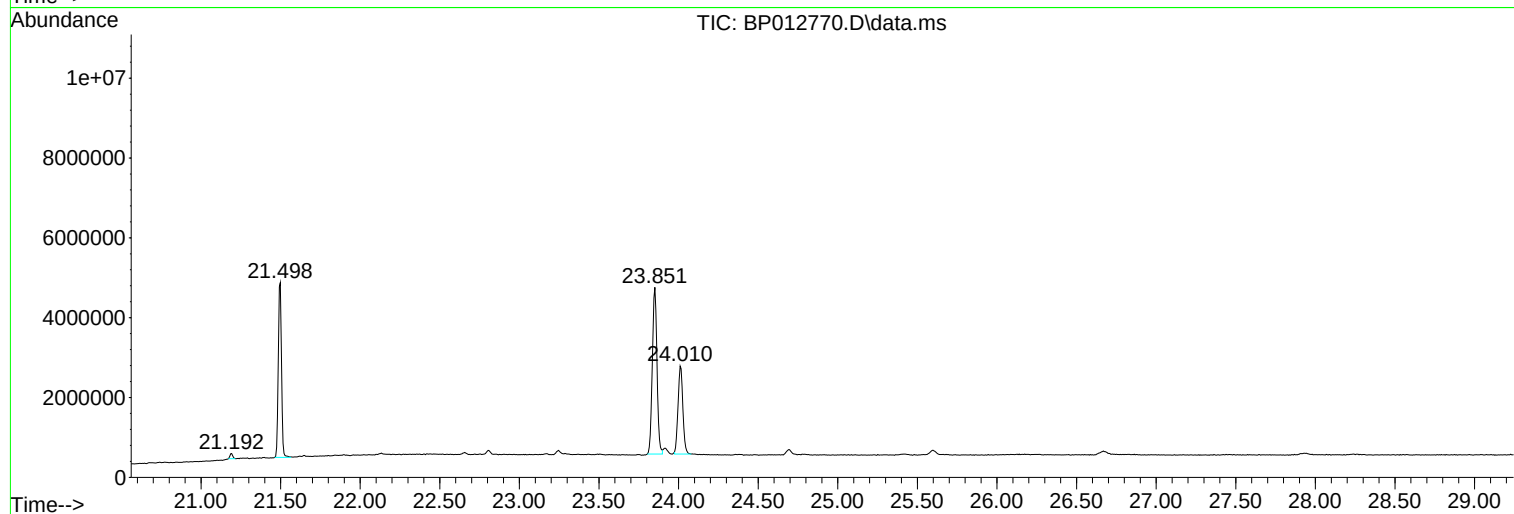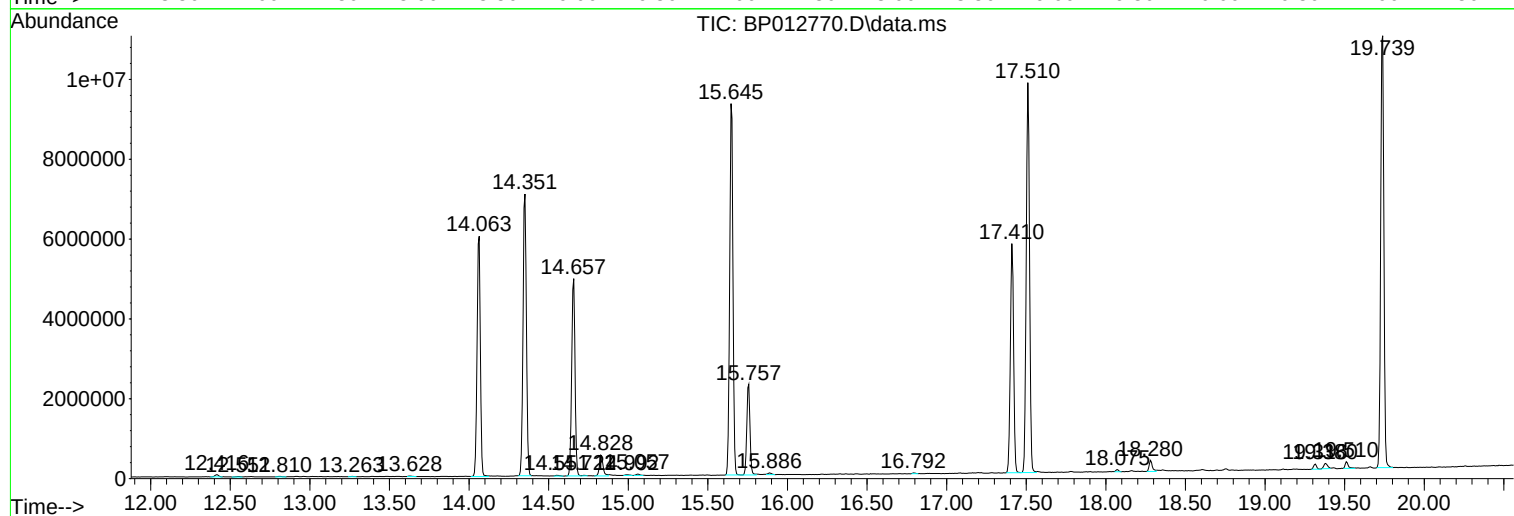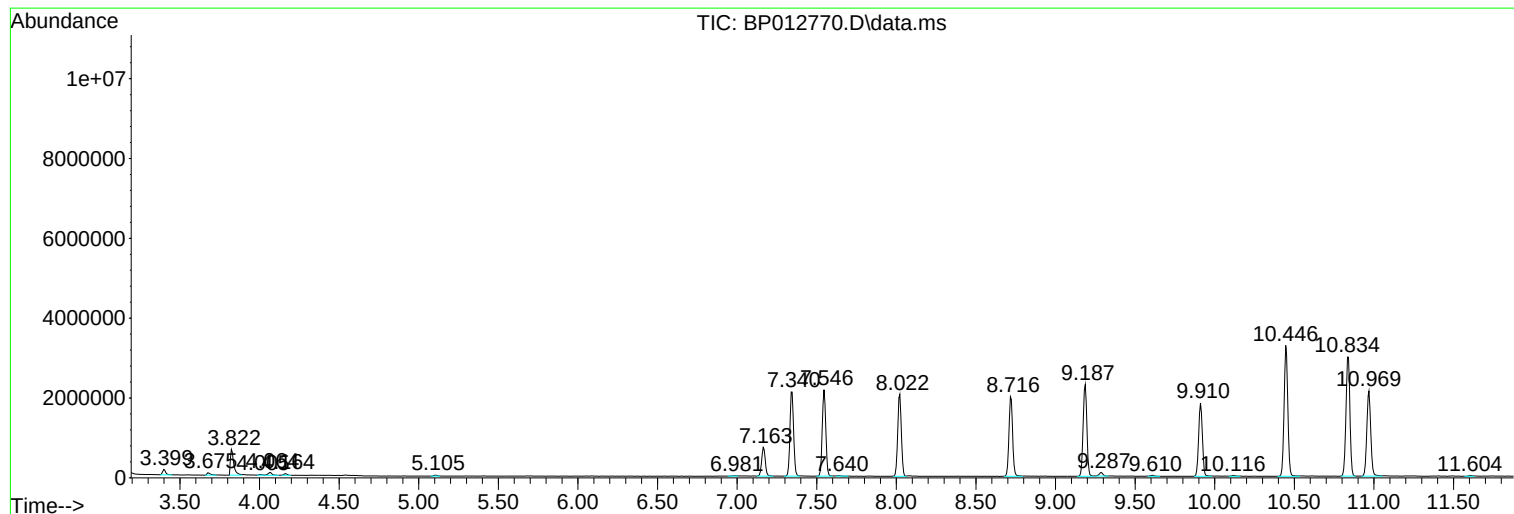

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012770.D
Acq On : 26 Nov 2022 16:27
Operator : CG/JU
Sample : N5602-11
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012770.D
Acq On : 26 Nov 2022 16:27
Operator : CG/JU
Sample : N5602-11
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
