

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012771.D
 Acq On : 26 Nov 2022 17:01
 Operator : CG/JU
 Sample : N5602-12
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012771.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	41	rBV	118841	157643	0.86%	0.098%
2	3.675	79	83	93	rBV	110156	169257	0.92%	0.106%
3	3.822	105	108	125	rBV	695844	1106152	6.04%	0.690%
4	4.064	144	149	155	rVB	59645	98612	0.54%	0.062%
5	4.164	161	166	172	rVB	33151	47547	0.26%	0.030%
6	5.105	320	326	332	rBV	33206	52394	0.29%	0.033%
7	5.281	351	356	362	rBV7	12445	21218	0.12%	0.013%
8	7.163	669	676	688	rBV	690926	1079442	5.90%	0.673%
9	7.340	699	706	716	rBV	2100640	3347160	18.28%	2.088%
10	7.546	730	741	749	rBV	2044156	3190363	17.42%	1.990%
11	7.634	751	756	761	rVB7	13085	28272	0.15%	0.018%
12	8.022	811	822	829	rBV	1835478	2944856	16.08%	1.837%
13	8.716	933	940	952	rBV	1904744	3023654	16.51%	1.886%
14	9.128	1004	1010	1012	rBV	18286	26111	0.14%	0.016%
15	9.187	1012	1020	1029	rVV	2327785	3812652	20.82%	2.378%
16	9.281	1031	1036	1041	rVB	36562	57442	0.31%	0.036%
17	9.610	1088	1092	1097	rVB3	17872	28663	0.16%	0.018%
18	9.910	1134	1143	1157	rBV	1827243	2964183	16.19%	1.849%
19	10.446	1227	1234	1248	rBV	3149940	5161026	28.19%	3.219%
20	10.604	1255	1261	1273	rBV	500120	811685	4.43%	0.506%
21	10.834	1292	1300	1310	rBV	2828207	4734203	25.86%	2.953%
22	10.969	1315	1323	1337	rBV	2179115	3832586	20.93%	2.391%
23	11.610	1426	1432	1435	rBV5	18711	32401	0.18%	0.020%
24	12.093	1510	1514	1521	rBV9	10372	19433	0.11%	0.012%
25	12.416	1563	1569	1574	rBV	59691	91345	0.50%	0.057%
26	13.016	1667	1671	1677	rBV8	12349	20254	0.11%	0.013%
27	13.263	1711	1713	1720	rVB6	15058	24004	0.13%	0.015%
28	13.551	1756	1762	1767	rVV	331264	498052	2.72%	0.311%
29	13.622	1771	1774	1778	rVB5	13516	21400	0.12%	0.013%
30	14.063	1841	1849	1858	rBV	6144739	8833023	48.24%	5.510%
31	14.192	1866	1871	1877	rVB9	23985	48922	0.27%	0.031%
32	14.292	1884	1888	1891	rBV5	35886	55635	0.30%	0.035%
33	14.351	1891	1898	1909	rVB	6925050	10496695	57.33%	6.548%
34	14.563	1930	1934	1941	rVB5	38488	70031	0.38%	0.044%
35	14.657	1943	1950	1958	rVV	4647695	6866259	37.50%	4.283%
36	14.834	1973	1980	1986	rBV	591505	926341	5.06%	0.578%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012771.D
 Acq On : 26 Nov 2022 17:01
 Operator : CG/JU
 Sample : N5602-12
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	14.992	2002	2007	2011	rBV3	47721	90763	0.50%	0.057%
38	15.057	2016	2018	2022	rVB4	29191	36357	0.20%	0.023%
39	15.645	2112	2118	2131	rBV	9438483	13656860	74.59%	8.519%
40	15.757	2131	2137	2145	rBV	2540086	3467637	18.94%	2.163%
41	15.828	2146	2149	2154	rVB	51177	71222	0.39%	0.044%
42	17.410	2412	2418	2425	rBV	5845833	8279568	45.22%	5.165%
43	17.510	2429	2435	2443	rVV	10580389	14778554	80.72%	9.219%
44	18.069	2527	2530	2536	rVB	200351	261943	1.43%	0.163%
45	18.280	2562	2566	2575	rBV	543120	810755	4.43%	0.506%
46	19.198	2719	2722	2726	rVB	430682	465735	2.54%	0.291%
47	19.327	2738	2744	2748	rBV2	265531	437991	2.39%	0.273%
48	19.374	2749	2752	2758	rVB	163662	264145	1.44%	0.165%
49	19.510	2772	2775	2788	rBV	327597	463530	2.53%	0.289%
50	19.739	2808	2814	2827	rVB	13630443	18309356	100.00%	11.421%
51	20.222	2894	2896	2899	rBV4	85902	85053	0.46%	0.053%
52	20.580	2953	2957	2961	rVB2	305382	358558	1.96%	0.224%
53	21.192	3058	3061	3067	rVB2	233848	279958	1.53%	0.175%
54	21.498	3107	3113	3124	rBV	6603700	8946789	48.86%	5.581%
55	23.851	3505	3513	3521	rBV2	8061097	16239853	88.70%	10.130%
56	24.015	3533	3541	3555	rVB2	3937809	8307250	45.37%	5.182%




Sum of corrected areas: 160310793

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012771.D
Acq On : 26 Nov 2022 17:01
Operator : CG/JU
Sample : N5602-12
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

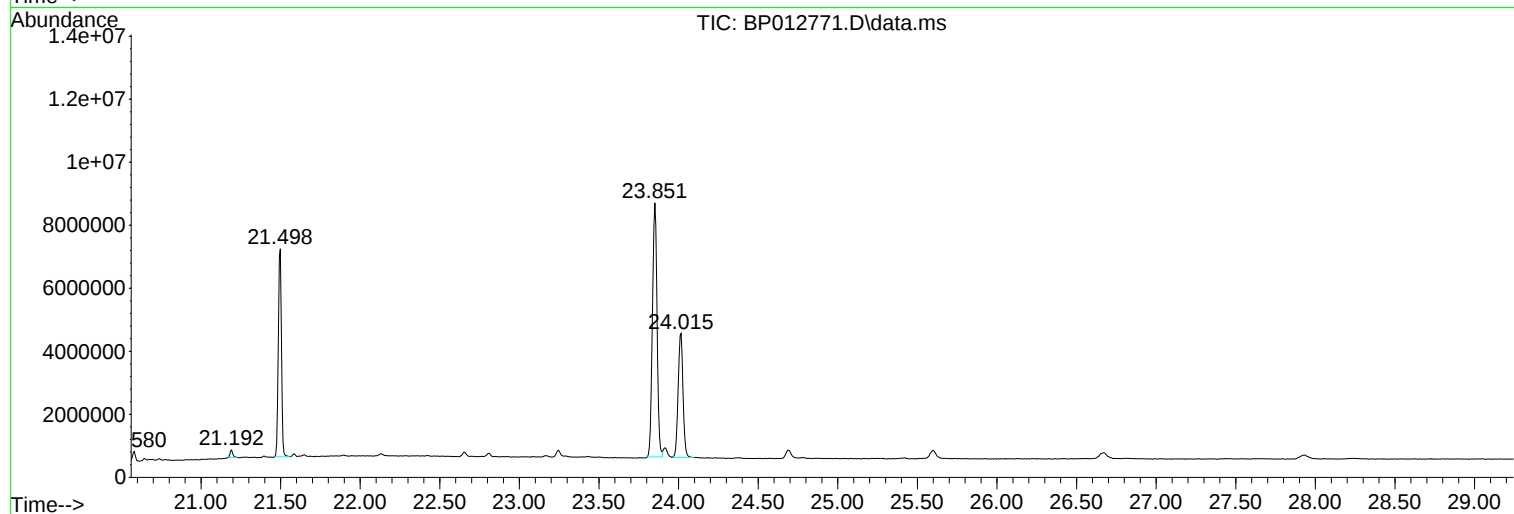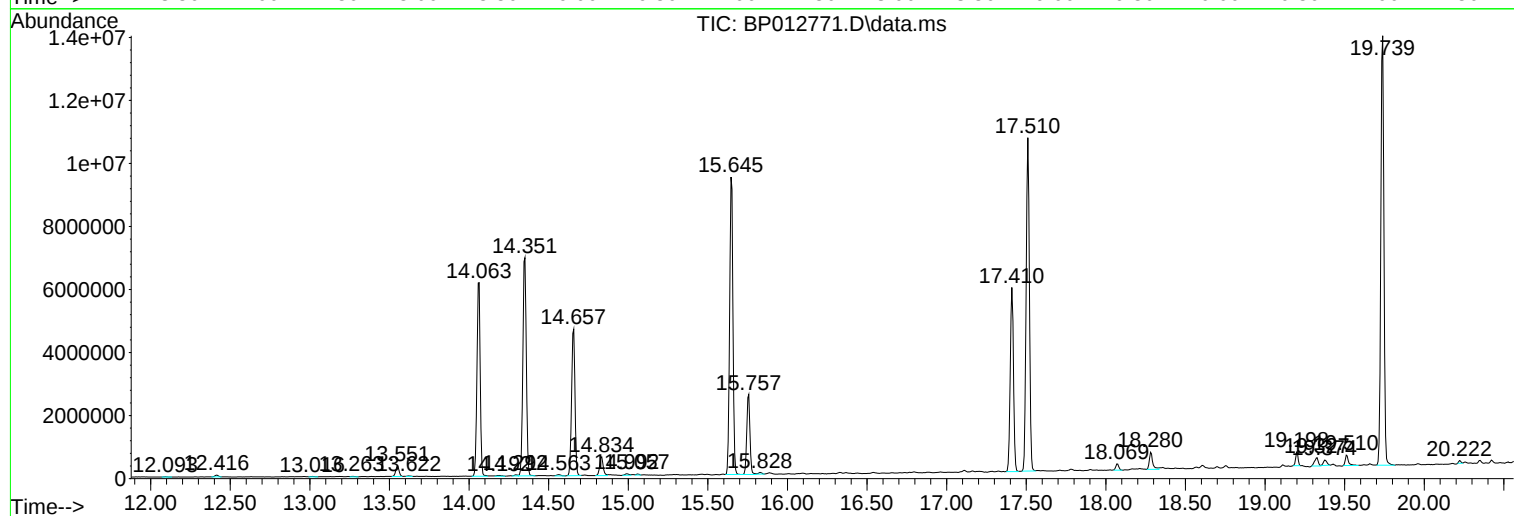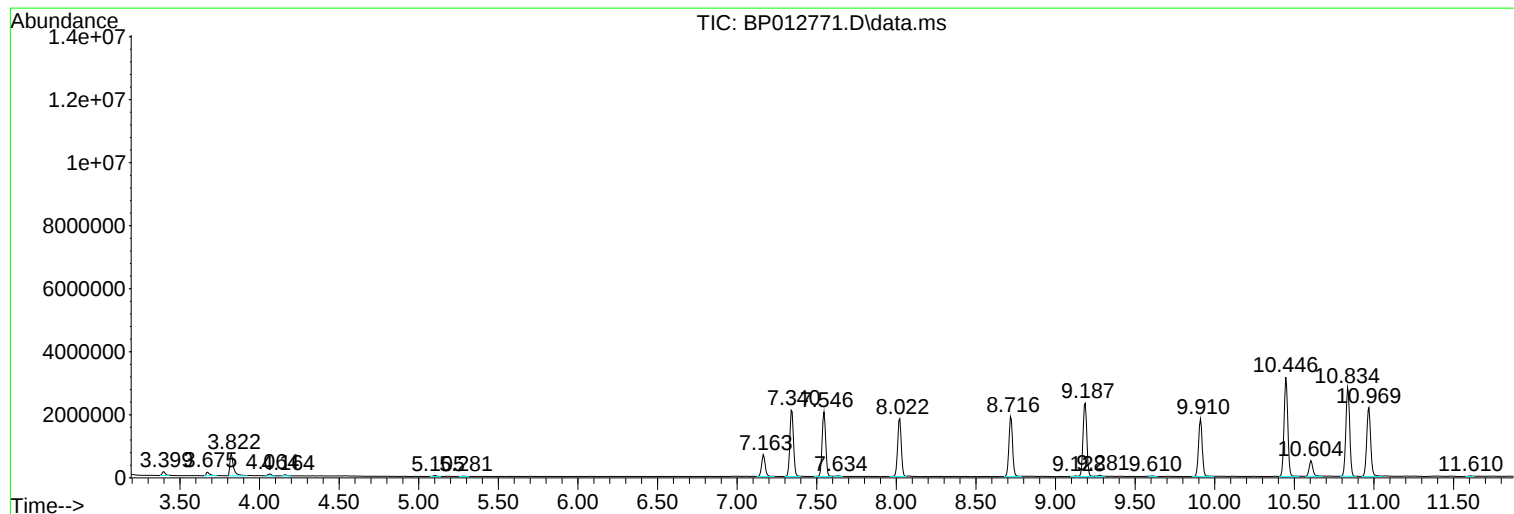

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012771.D
Acq On : 26 Nov 2022 17:01
Operator : CG/JU
Sample : N5602-12
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.604	3.43 ng/ul	811685	Naphthalene-d8	10.834

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	74
4			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	72
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	72

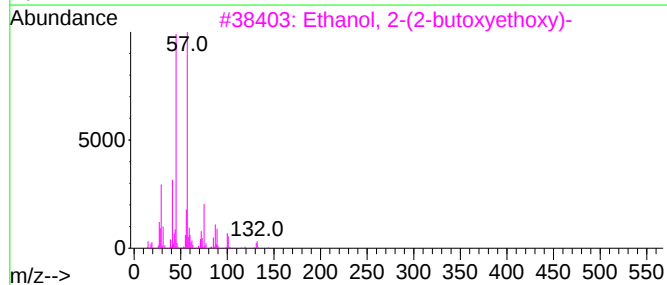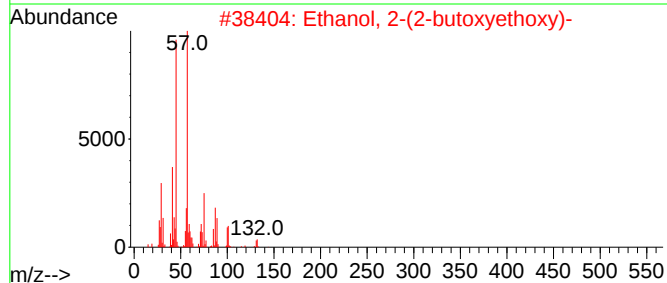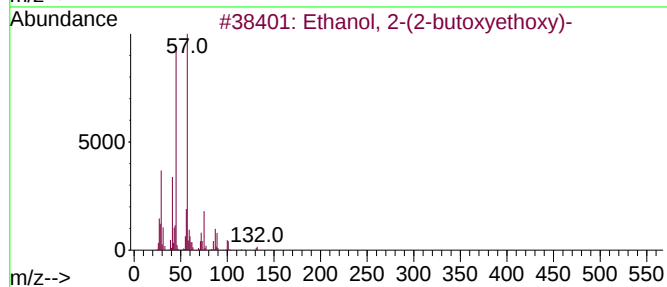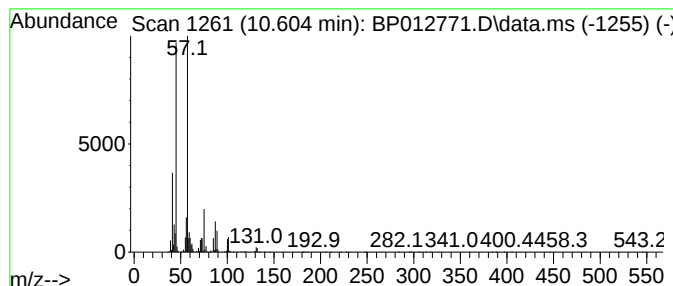

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012771.D
Acq On : 26 Nov 2022 17:01
Operator : CG/JU
Sample : N5602-12
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.604	3.4	ng/u1	811685	2	10.834	4734200	20.0