

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012774.D
 Acq On : 26 Nov 2022 18:43
 Operator : CG/JU
 Sample : N5602-03
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012774.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	46	rVB	117989	175328	0.95%	0.112%
2	3.669	78	82	95	rBV	504086	707050	3.83%	0.453%
3	3.822	105	108	124	rBV	695574	1097146	5.94%	0.702%
4	4.064	144	149	160	rVB2	55978	98177	0.53%	0.063%
5	4.158	161	165	174	rVB	34321	57032	0.31%	0.037%
6	4.381	199	203	207	rVB4	31016	42981	0.23%	0.028%
7	4.805	269	275	278	rVB4	19830	29511	0.16%	0.019%
8	5.099	320	325	336	rVB	173420	262796	1.42%	0.168%
9	6.081	488	492	500	rVB2	12815	22709	0.12%	0.015%
10	7.163	670	676	687	rVB	627945	981637	5.31%	0.628%
11	7.340	698	706	715	rBV	2044681	3226250	17.46%	2.065%
12	7.410	715	718	724	rVB	13109	20255	0.11%	0.013%
13	7.546	733	741	753	rBV	1948812	3060713	16.56%	1.959%
14	7.634	753	756	760	rVB5	12626	18499	0.10%	0.012%
15	8.016	813	821	828	rBV	1762576	2839649	15.37%	1.818%
16	8.081	828	832	842	rVB	28768	48774	0.26%	0.031%
17	8.716	933	940	950	rBV	1705365	2733367	14.79%	1.750%
18	9.181	1011	1019	1030	rBV	2228206	3679439	19.91%	2.355%
19	9.275	1030	1035	1040	rVB6	12550	24377	0.13%	0.016%
20	9.610	1084	1092	1096	rVB	33011	53588	0.29%	0.034%
21	9.910	1132	1143	1156	rBV	1786030	2867688	15.52%	1.836%
22	10.446	1226	1234	1248	rBV	2978737	4849770	26.24%	3.104%
23	10.834	1292	1300	1309	rBV	2669839	4487596	24.28%	2.872%
24	10.969	1315	1323	1340	rBV	2105668	3680423	19.92%	2.356%
25	11.604	1427	1431	1435	rBV6	12465	21402	0.12%	0.014%
26	12.416	1561	1569	1575	rVB	53452	89459	0.48%	0.057%
27	12.640	1600	1607	1612	rBV5	9059	19276	0.10%	0.012%
28	13.481	1746	1750	1755	rVB2	18487	25478	0.14%	0.016%
29	13.551	1757	1762	1766	rVV2	15069	23775	0.13%	0.015%
30	13.616	1766	1773	1781	rVB8	19404	40113	0.22%	0.026%
31	14.057	1841	1848	1863	rBV	6067264	8512558	46.07%	5.449%
32	14.175	1863	1868	1873	rVB8	12177	19675	0.11%	0.013%
33	14.351	1891	1898	1908	rVV	6799601	10243205	55.43%	6.557%
34	14.434	1910	1912	1921	rVB10	9930	20627	0.11%	0.013%
35	14.551	1928	1932	1936	rVB3	20552	27721	0.15%	0.018%
36	14.604	1936	1941	1943	rBV	23266	32032	0.17%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
 Data File : BP012774.D
 Acq On : 26 Nov 2022 18:43
 Operator : CG/JU
 Sample : N5602-03
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AF5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	14.657	1943	1950	1957	rVV	4395569	6581720	35.62%	4.213%
38	14.828	1973	1979	1992	rBV	593422	946374	5.12%	0.606%
39	14.992	2002	2007	2013	rBV9	16083	34297	0.19%	0.022%
40	15.057	2013	2018	2023	rVB6	28804	48706	0.26%	0.031%
41	15.504	2090	2094	2098	rVB3	16366	23090	0.12%	0.015%
42	15.645	2111	2118	2130	rBV	9074014	13397207	72.50%	8.575%
43	15.757	2130	2137	2148	rVV	2411724	3360941	18.19%	2.151%
44	15.886	2155	2159	2167	rVB2	43902	69743	0.38%	0.045%
45	16.363	2237	2240	2245	rBV4	15865	23195	0.13%	0.015%
46	16.422	2247	2250	2258	rVB5	15827	34721	0.19%	0.022%
47	16.792	2309	2313	2317	rBV4	29866	41986	0.23%	0.027%
48	16.863	2321	2325	2330	rVV7	11187	18552	0.10%	0.012%
49	17.410	2411	2418	2424	rBV	5727962	8048764	43.56%	5.152%
50	17.510	2429	2435	2444	rBV2	10233583	14668697	79.38%	9.389%
51	17.628	2453	2455	2463	rVB	18716	24456	0.13%	0.016%
52	17.775	2478	2480	2486	rVB3	18654	28450	0.15%	0.018%
53	18.075	2526	2531	2536	rVB	89374	109530	0.59%	0.070%
54	18.157	2541	2545	2551	rBV8	24581	39733	0.22%	0.025%
55	18.280	2561	2566	2574	rBV	324419	456595	2.47%	0.292%
56	18.351	2576	2578	2585	rVB2	24810	41499	0.22%	0.027%
57	18.698	2634	2637	2641	rVB4	32070	38524	0.21%	0.025%
58	18.751	2643	2646	2650	rVV5	34484	44344	0.24%	0.028%
59	19.151	2709	2714	2719	rBV	86262	127242	0.69%	0.081%
60	19.316	2737	2742	2747	rBV2	151340	229246	1.24%	0.147%
61	19.380	2748	2753	2759	rBV	162916	283781	1.54%	0.182%
62	19.510	2771	2775	2780	rBV2	148444	195504	1.06%	0.125%
63	19.663	2798	2801	2804	rBV3	32965	34390	0.19%	0.022%
64	19.739	2807	2814	2825	rBV	13631420	18479233	100.00%	11.828%
65	21.186	3056	3060	3071	rBV2	511710	791566	4.28%	0.507%
66	21.498	3107	3113	3124	rBV	6386118	8761496	47.41%	5.608%
67	22.804	3331	3335	3340	rBV	415586	605416	3.28%	0.388%
68	23.851	3505	3513	3521	rBV2	7982034	16432005	88.92%	10.518%
69	24.015	3533	3541	3556	rVB2	3828422	8067251	43.66%	5.164%




Sum of corrected areas: 156228330

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012774.D
Acq On : 26 Nov 2022 18:43
Operator : CG/JU
Sample : N5602-03
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

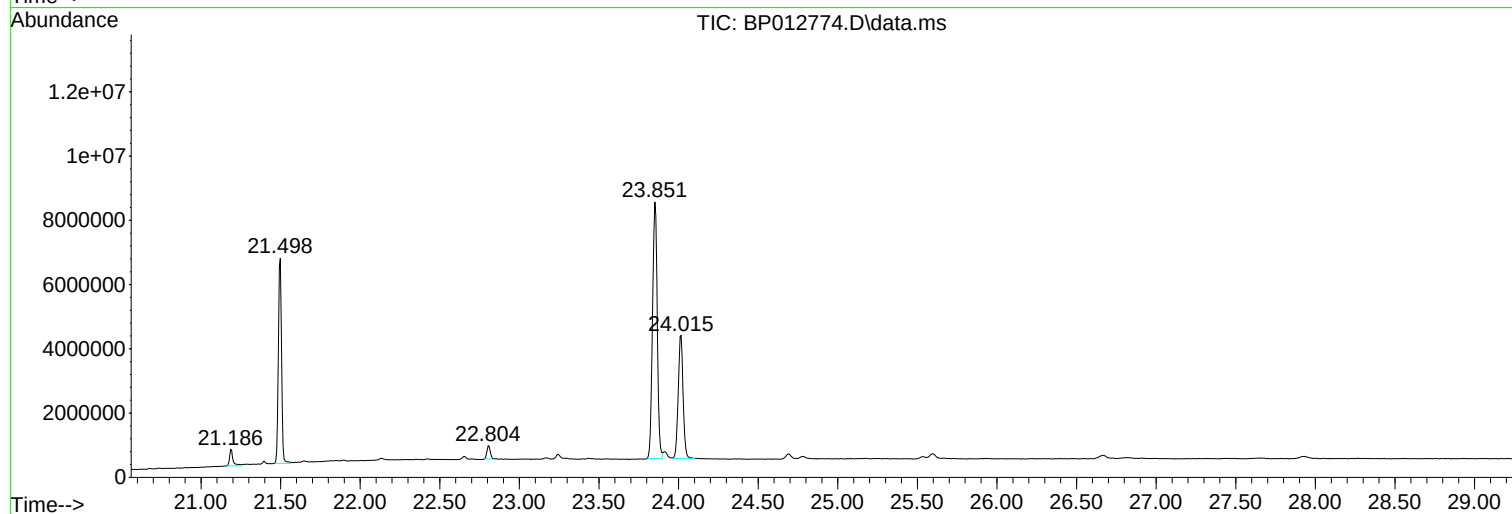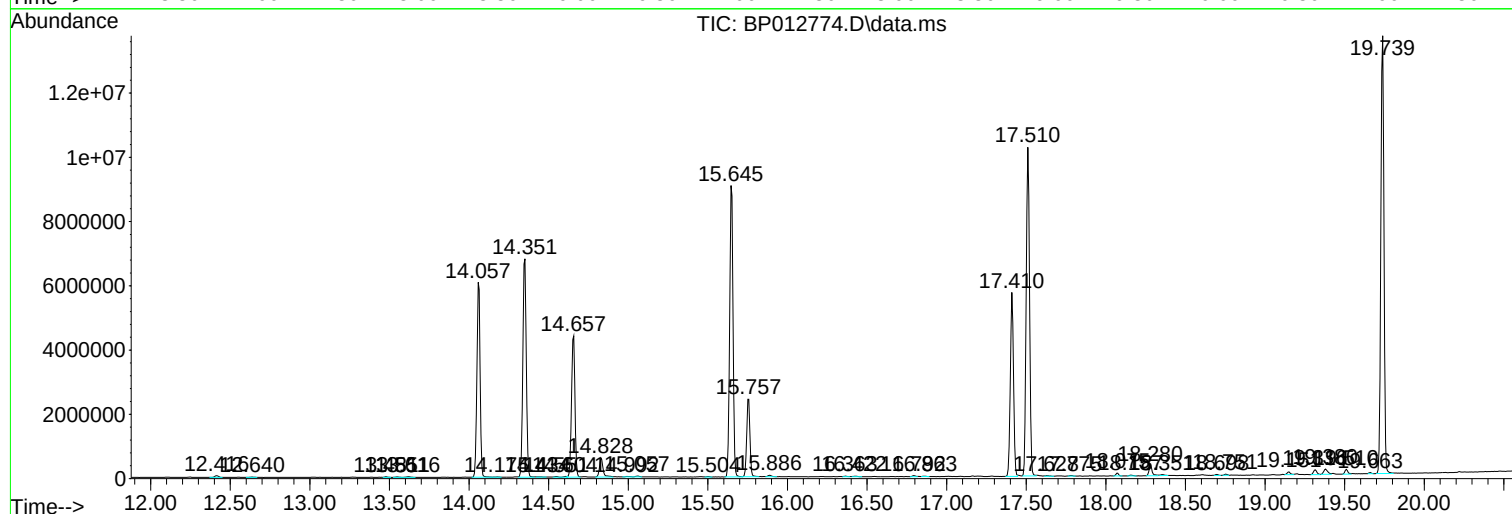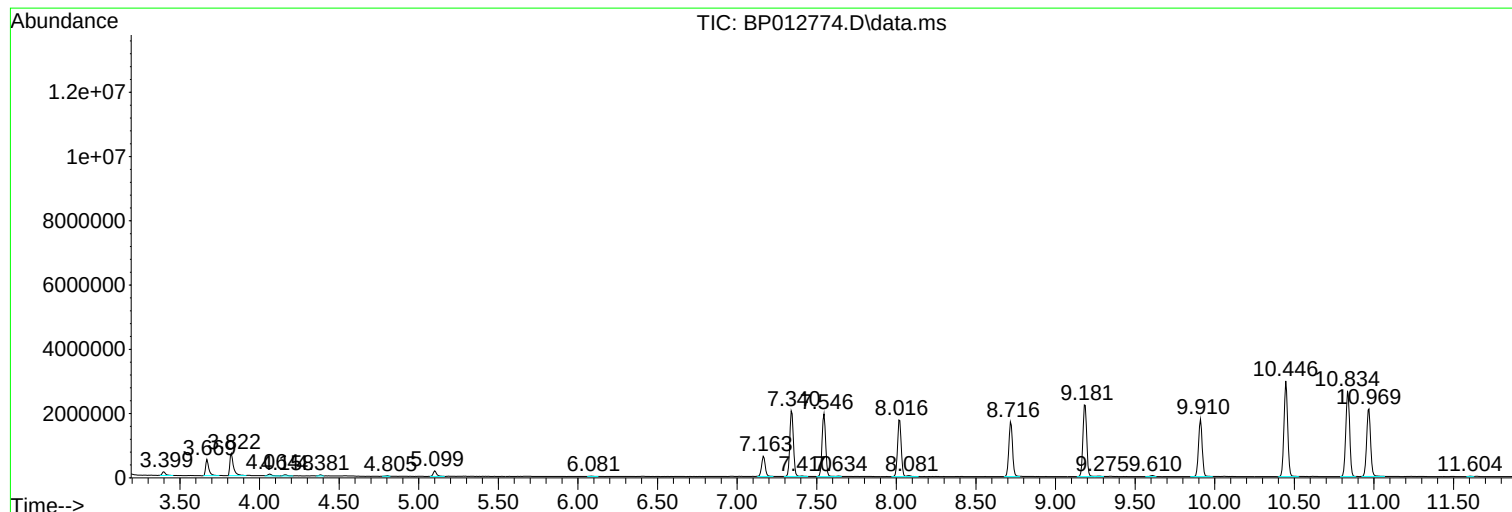

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012774.D
Acq On : 26 Nov 2022 18:43
Operator : CG/JU
Sample : N5602-03
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propylene Glycol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.669	4.98 ng/ul	707050	1,4-Dichlorobenzene-d4	8.022

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propylene Glycol	76	C3H8O2	000057-55-6	90
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
3			(S)-(+)-1,2-Propanediol	76	C3H8O2	004254-15-3	43
4			Propanoic acid, 2-hydroxy-, meth...	104	C4H8O3	000547-64-8	40
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	9

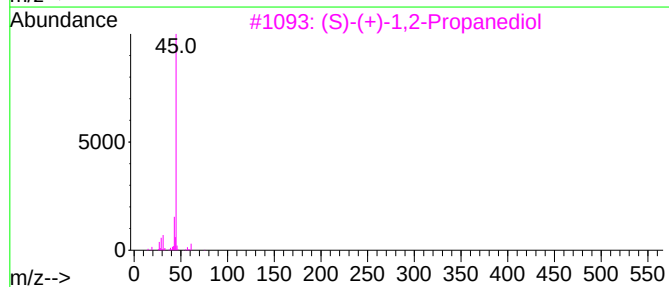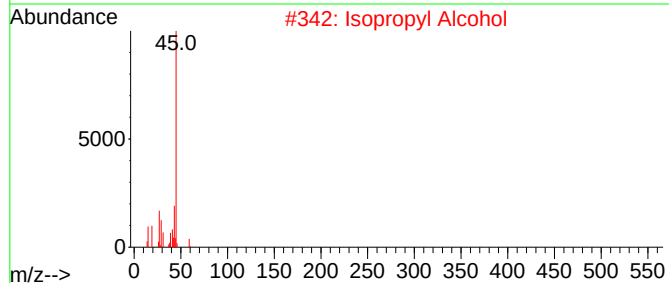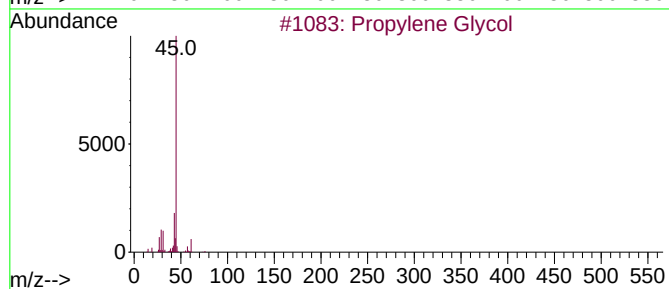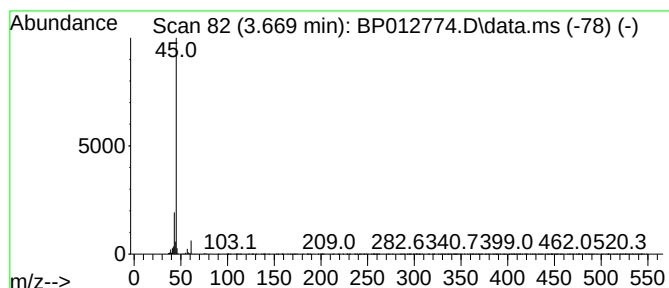

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112522\
Data File : BP012774.D
Acq On : 26 Nov 2022 18:43
Operator : CG/JU
Sample : N5602-03
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propylene Glycol	3.669	5.0	ng/u1	707050	1	8.022	2839650	20.0